



**APEX BIO**  
Achieve Perfection, Explore the Unknown

# Mass Spectrometry

## 1. Analysis Information

Product Name:	Gap 26
Operator:	David
Injection Date:	11/27/2017 3:47:59 PM
Inj. Volume:	1
Batch No.:	2

## 2. Acquisition Parameter


Probe:	ESI
Gas Temp:	350°C
Gas Flow:	11L/min
Nebulizer:	50psi
VCap:	4000v
Fragmentor:	70v
Reference:	m/z 121.050873, 922.009798
T.Flow:	0.3ml/min
B.conc:	20%H <sub>2</sub> O/80%ACN

## 3. Result

NT-S20171127-031

20171127-197250-15-0-F 16 (0.269)

1: Scan ES+  
1.14e8

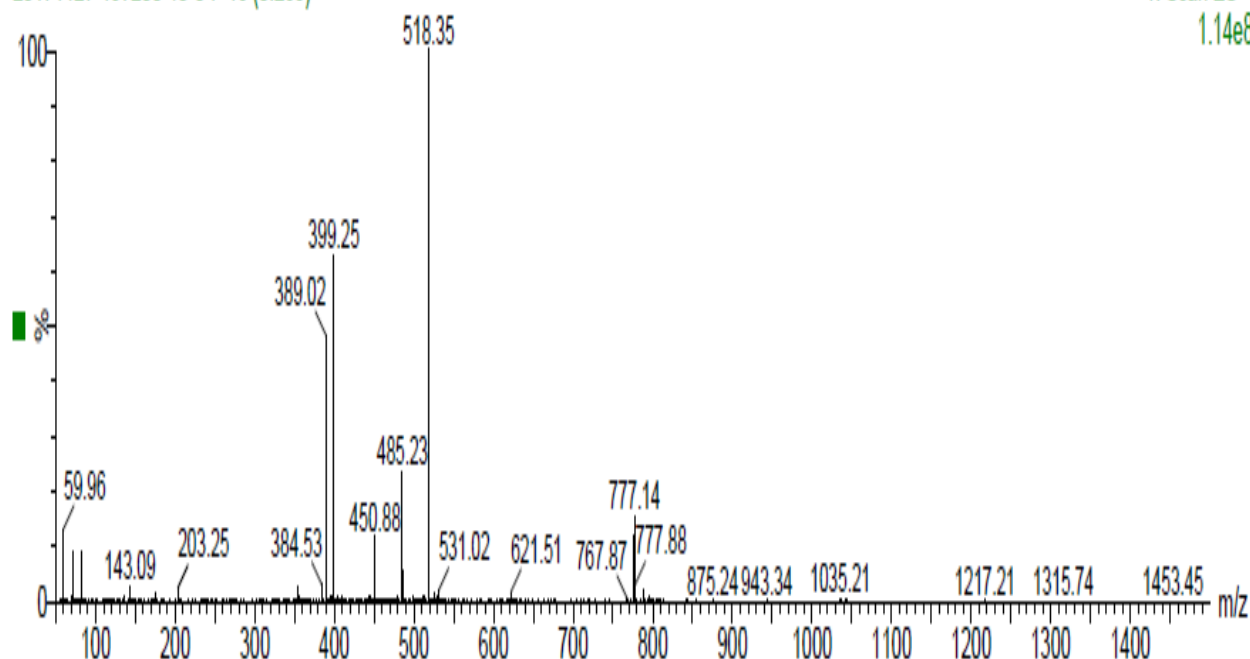

Molecular Weight:	1550.79
m/z([M+3H] <sup>3+</sup> ) Base Peak :	518.35
m/z([M+4H] <sup>4+</sup> ) Base Peak :	389.02