

High Performance Liquid Chromatography

Analysis Information

Product Name: type II collagen fragment

Operator: David

Injection Date: 2/16/2019 6:38:59 PM

Batch No.: 1

HPLC Condition

Column : ZORBAX Eclipse Pluse C18 3.5 μ m 4.6mmx100mm

Solvent A: H2O+0.1%TFA

Solvent B: ACN+0.1%TFA

Gradient:

Time	A	B
0.0min	95%	5%
2.0min	95%	5%
7.0min	5%	95%
10.00min	0%	100%
12.00min	0%	100%
12.10min	95%	5%
15.00min	Stop	Stop


Flow rate: 1mL/min

Wavelength: 220nm

Volume:

10µl

Result

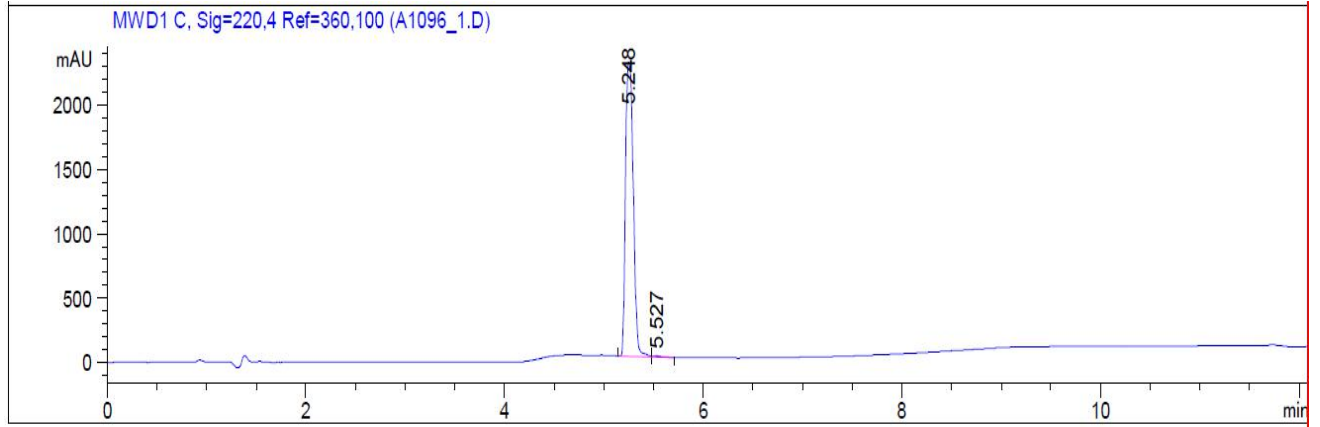

Rank	RetTime(min)	Area(mAU*s)	Area %
1	5.248	1.24924e4	99.5691
2	5.527	54.06136	0.4309

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com