

1. Analysis Information

Product Name:	E-64
Operator:	David
Injection Date:	12/26/2016 01:22:18 PM
Inj. Volume:	1
Batch No.:	2


2. Acquisition Parameter

Probe:	ESI
Gas Temp:	350°C
Gas Flow:	11L/min
Nebulizer:	50psi
VCap:	4000v
Fragmentor:	70v
Reference:	m/z 121.050873, 922.009798
T.Flow:	0.3ml/min
B.conc:	20%H ₂ O/80%ACN

3. Result

20161226-B1-1223 10 (0.174)

2: Scan ES-
2.27e7

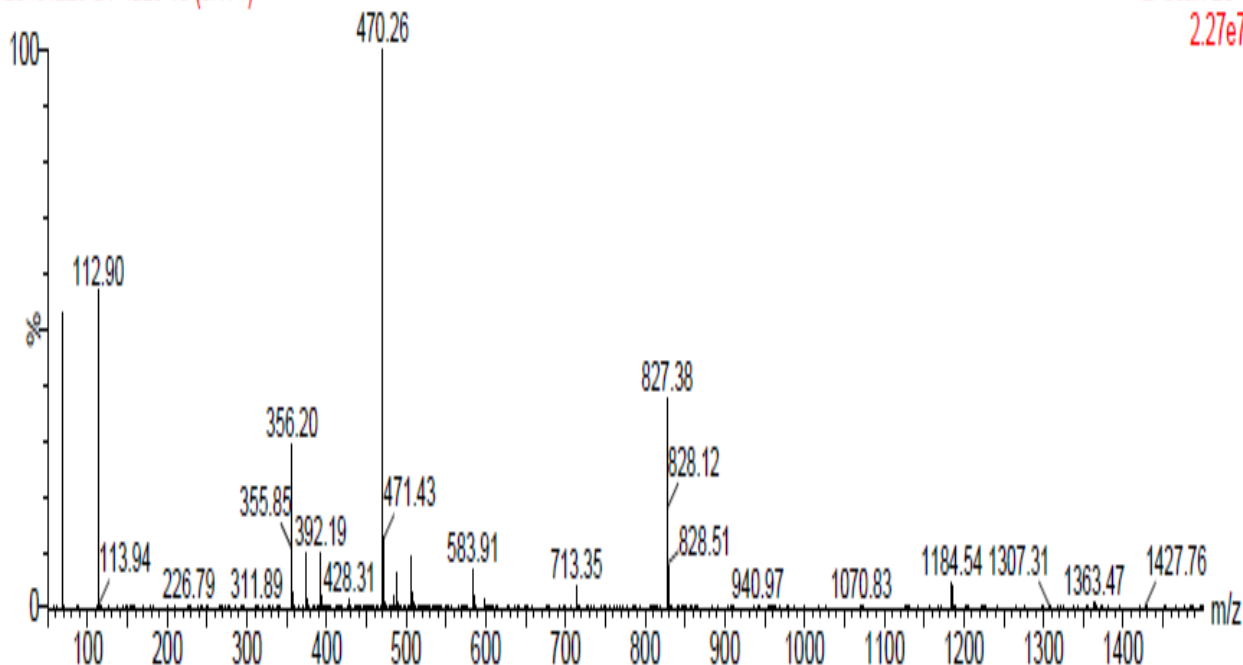

Molecular Weight:	357.41
m/z(M-2H) Base Peak :	355.20
m/z(M-H) Base Peak :	356.20