

1. Analysis Information

Product Name:	E-64
Operator:	David
Injection Date:	12/26/2016 14:59:59 PM
Inj. Volume:	1
Batch No.:	3


2. Acquisition Parameter

Probe:	ESI
Gas Temp:	350°C
Gas Flow:	11L/min
Nebulizer:	50psi
VCap:	4000v
Fragmentor:	70v
Reference:	m/z 121.050873, 922.009798
T.Flow:	0.3ml/min
B.conc:	20%H ₂ O/80%ACN

3. Result

20161226-B1-1223 10 (0.165)

1: Scan ES+
6.23e7

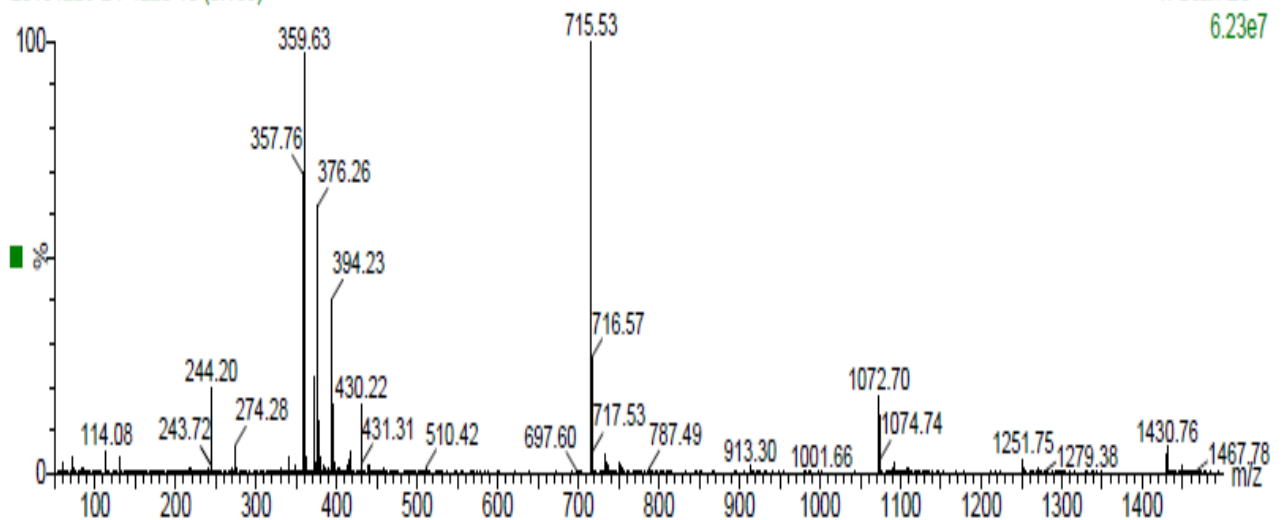

Molecular Weight:	357.41
m/z(M) Base Peak :	357.76