

High Performance Liquid Chromatography


1. Analysis Information

Product Name:	OSI-930
Operator:	David
Injection Date:	11/20/2017 3:54:53 PM
Batch No.:	2

2. HPLC Condition

Column:	Athena C18, 3 μ m, 2.1mm \times 100 mm																
Solvent A:	0.1% H3PO4 in 100% Acetonitrile																
Solvent B:	0.1% H3PO4 in 100% Water																
Gradient:	<table border="1"> <thead> <tr> <th>Time</th> <th>A</th> <th>B</th> </tr> </thead> <tbody> <tr> <td>0.0min</td> <td>10%</td> <td>90%</td> </tr> <tr> <td>6.0min</td> <td>95%</td> <td>5%</td> </tr> <tr> <td>10.0 min</td> <td>95%</td> <td>5%</td> </tr> <tr> <td>10.0min</td> <td>Stop</td> <td>Stop</td> </tr> </tbody> </table>		Time	A	B	0.0min	10%	90%	6.0min	95%	5%	10.0 min	95%	5%	10.0min	Stop	Stop
Time	A	B															
0.0min	10%	90%															
6.0min	95%	5%															
10.0 min	95%	5%															
10.0min	Stop	Stop															
Flow rate:	0.45ml/min																
Wavelength:	230nm																
Volume:	10 μ l																

3. Result

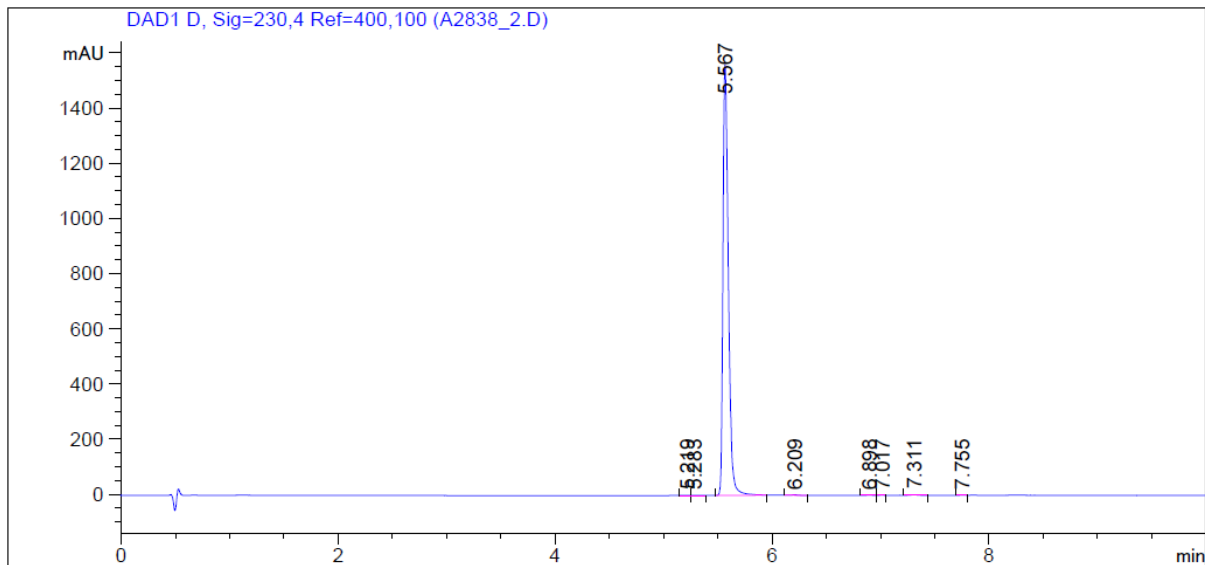

Rank	RetTime(min)	Area(mAU*s)	Area %
1	5.219	3.46902	0.0638
2	5.283	3.59818	0.0662
3	5.567	5407.81592	99.4658
4	6.209	6.65545	0.1224
5	6.898	2.71722	0.0500
6	7.017	1.69494	0.0312
7	7.311	9.83815	0.1810
8	7.755	1.07100	0.0197