

1. Analysis Information

Product Name:	AM095
Operator:	David
Injection Date:	1/31/2018 3:28:34 PM
Inj. Volume:	1
Batch No.:	2


2. Acquisition Parameter

Probe:	ESI
Gas Temp:	350°C
Gas Flow:	11L/min
Nebulizer:	50psi
VCap:	4000v
Fragmentor:	70v
Reference:	m/z 121.050873, 922.009798
T.Flow:	0.3ml/min
B.conc:	20%H ₂ O/80%ACN

3. Result

20180131-1345614-59-6-F 9 (0.156)

2: Scan ES-
6.62e7

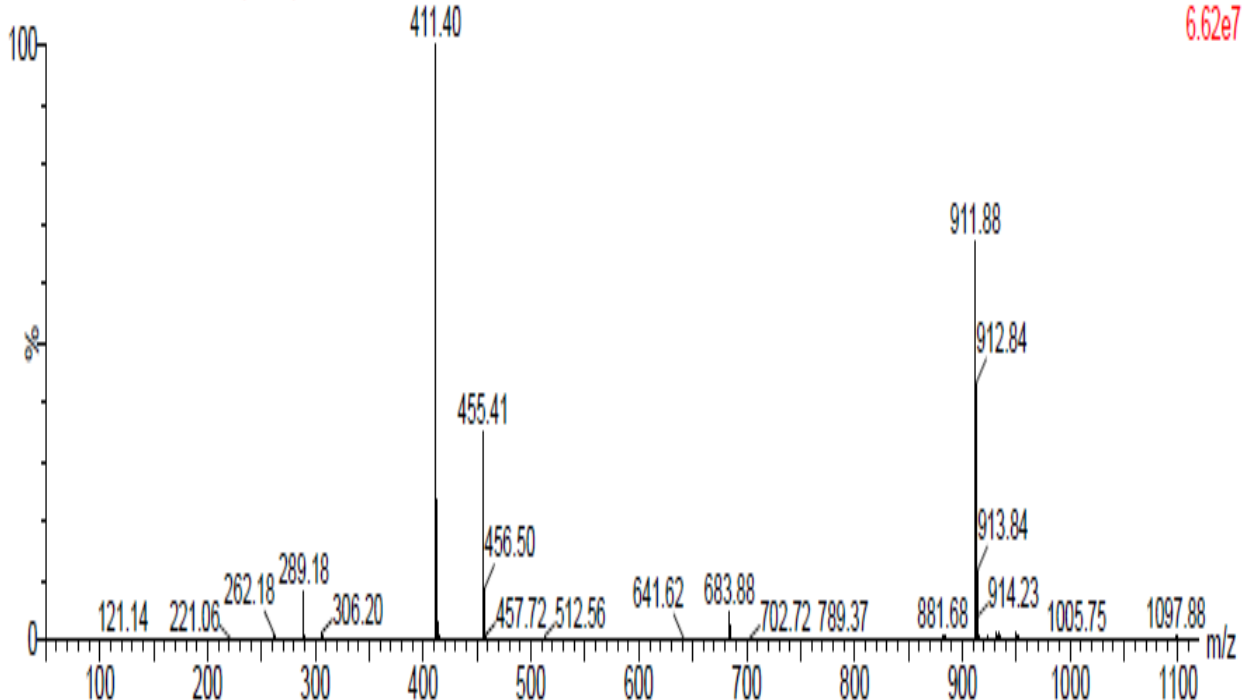

Molecular Weight:	478.47
m/z(M-Na) Base Peak :	455.41