

High Performance Liquid Chromatography

1. Analysis Information

Product Name:	AM-095 free base
Operator:	David
Injection Date:	7/28/2017 4:13:46 PM
Batch No.:	2


2. HPLC Condition

Column:	Athena C18, 3 μ m, 2.1mm \times 100 mm
Solvent A:	0.1% H ₃ PO ₄ in 100% Acetonitrile
Solvent B:	0.1% H ₃ PO ₄ in 100% Water

Gradient:	Time	A	B
	0.0min	0%	100%
	2.0min	0%	100%
	7.0min	95%	5%
	10.0min	95%	5%
	10.0min	Stop	Stop

Flow rate:	0.45ml/min
Wavelength:	280nm
Volume:	10 μ l

3. Result

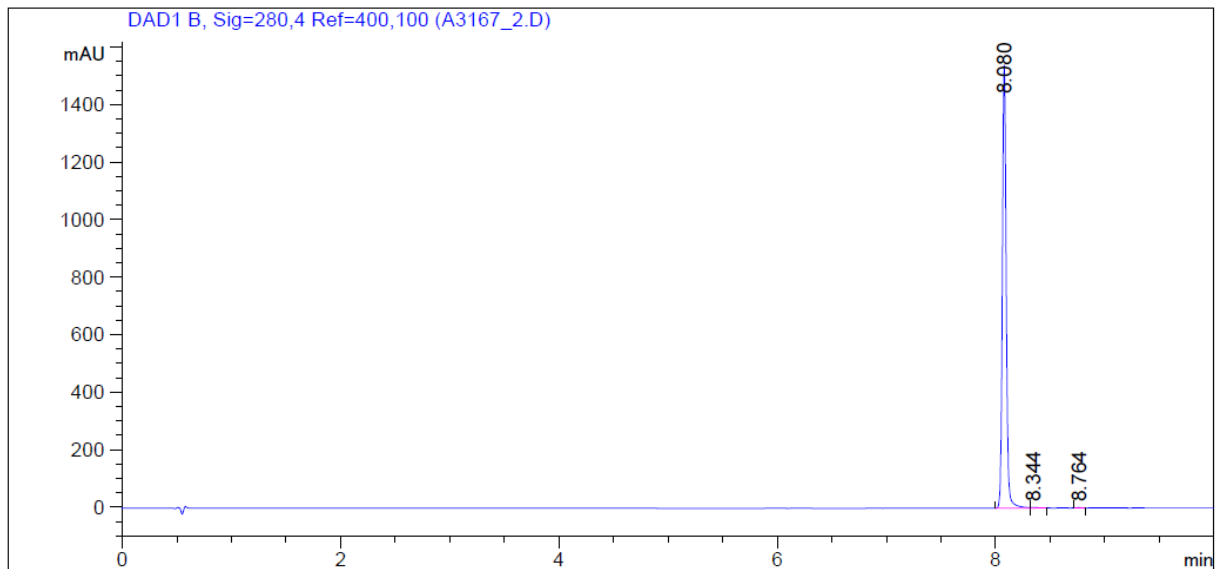

Rank	RetTime(min)	Area(mAU*s)	Area %
1	8.080	3804.10205	99.6985
2	8.344	8.05542	0.2111
3	8.764	3.44894	0.0904