

# High Performance Liquid Chromatography

## Analysis Information

**Product Name:** BMS-927711  
**Operator:** David  
**Injection Date:** 8/16/2022 14:17:12  
**Batch No.:** 2


## HPLC Condition

**Column :** ZORBAX Eclipse Pluse C18 3.5 $\mu$ m 4.6mmx100mm  
**Solvent A:** H2O+0.1%TFA  
**Solvent B:** ACN+0.1%TFA  
**Gradient:**

Time	A	B
0.0min	80%	20%
2.0min	80%	20%
7.0min	5%	95%
10.0min	0%	100%
12.0min	0%	100%
15.0min	Stop	Stop

**Flow rate:** 1ml/min  
**Wavelength:** 280nm  
**Volume:** 5 $\mu$ l

## Result

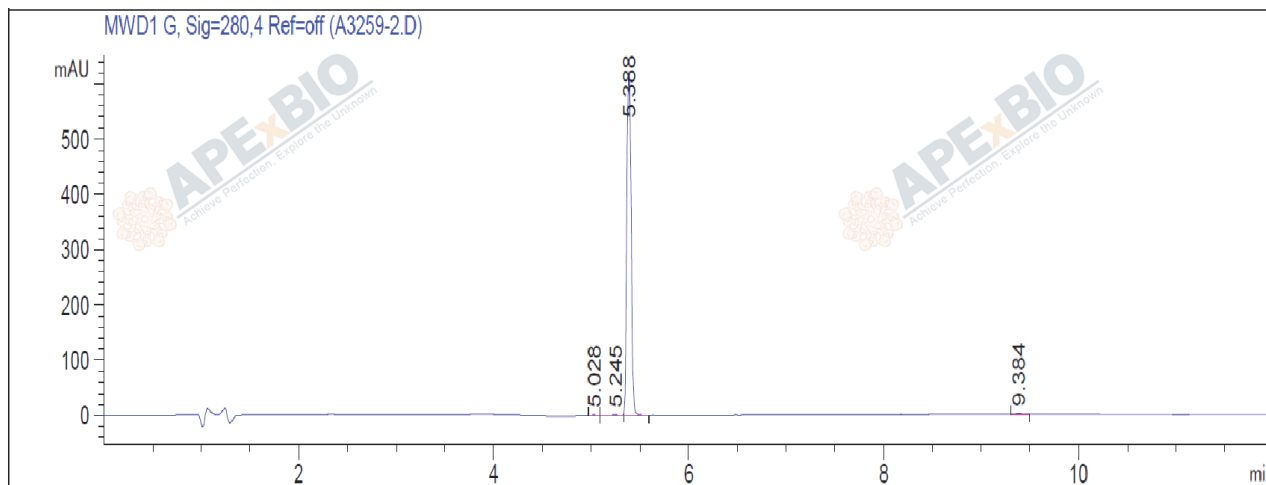

Rank	RetTime(min)	Area(mAU*s)	Area %
1	5.028	5.12015	0.2841
2	5.245	7.22476	0.4008
3	5.388	1784.36462	98.9944
4	9.384	5.78156	0.3208

## Caution

**FOR RESEARCH PURPOSES ONLY.**

**NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.**

**APEX BIO Technology**

**www.apexbt.com**

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com