

High Performance Liquid Chromatography

Analysis Information


Product Name: MK-4827
Operator: David
Injection Date: 8/30/2021 12:58:30 PM
Batch No.: 4

HPLC Condition

Column : Athena C18, 3 μ m, 2.1mm \times 100 mm
Solvent A: ACN+0.1%TFA
Solvent B: H2O+0.1%TFA
Gradient:

Time	A	B
0.0min	0%	100%
1.5min	0%	100%
6.0min	95%	5%
9.0min	95%	5%
9.0min	Stop	Stop

Flow rate: 0.46ml/min
Wavelength: 254nm
Volume: 3 μ l

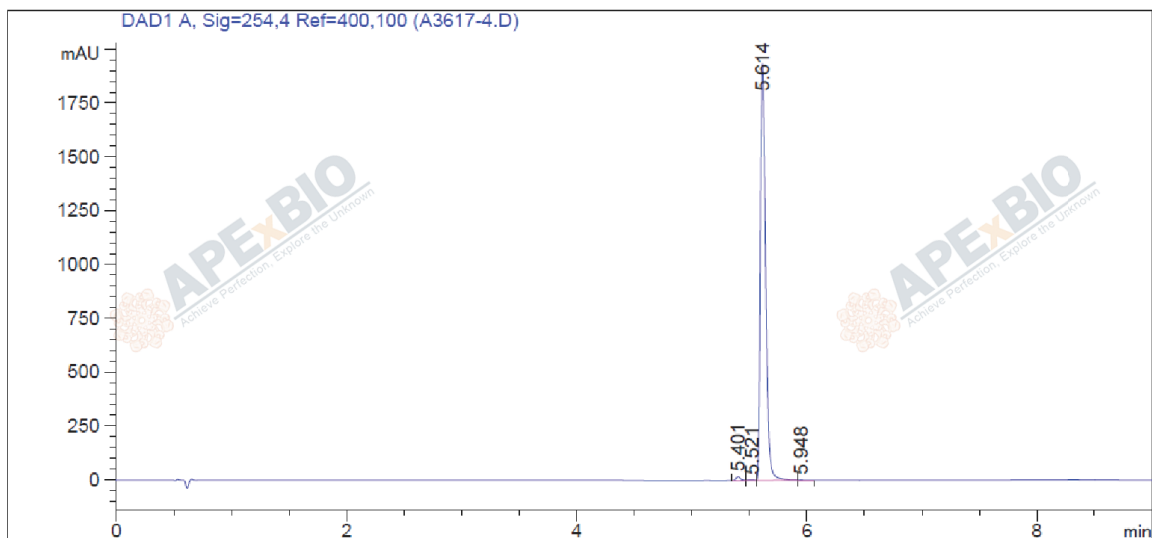

Rank	RetTime(min)	Area(mAU*s)	Area %
1	5.401	49.88733	0.7809
2	5.521	12.87158	0.2015
3	5.614	6320.14160	98.9351
4	5.948	5.26722	0.0825

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com