

High Performance Liquid Chromatography


1. Analysis Information

| | |
|-----------------|----------------------|
| Product Name: | OTX-015 |
| Operator: | David |
| Injection Date: | 4/13/2018 1:57:19 PM |
| Batch No.: | 5 |

2. HPLC Condition

| Column: | Athena C18, 3 μ m, 2.1mm \times 100 mm | | | | | | | | | | | | | | | | | | | |
|-------------|--|------|------|---|---|--------|----|------|--------|----|------|--------|-----|----|----------|-----|----|---------|------|------|
| Solvent A: | 0.1% H ₃ PO ₄ in 100% Acetonitrile | | | | | | | | | | | | | | | | | | | |
| Solvent B: | 0.1% H ₃ PO ₄ in 100% Water | | | | | | | | | | | | | | | | | | | |
| Gradient: | <table border="1"> <thead> <tr> <th>Time</th> <th>A</th> <th>B</th> </tr> </thead> <tbody> <tr> <td>0.0min</td> <td>0%</td> <td>100%</td> </tr> <tr> <td>2.0min</td> <td>0%</td> <td>100%</td> </tr> <tr> <td>7.0min</td> <td>95%</td> <td>5%</td> </tr> <tr> <td>10.0 min</td> <td>95%</td> <td>5%</td> </tr> <tr> <td>10.0min</td> <td>Stop</td> <td>Stop</td> </tr> </tbody> </table> | | Time | A | B | 0.0min | 0% | 100% | 2.0min | 0% | 100% | 7.0min | 95% | 5% | 10.0 min | 95% | 5% | 10.0min | Stop | Stop |
| Time | A | B | | | | | | | | | | | | | | | | | | |
| 0.0min | 0% | 100% | | | | | | | | | | | | | | | | | | |
| 2.0min | 0% | 100% | | | | | | | | | | | | | | | | | | |
| 7.0min | 95% | 5% | | | | | | | | | | | | | | | | | | |
| 10.0 min | 95% | 5% | | | | | | | | | | | | | | | | | | |
| 10.0min | Stop | Stop | | | | | | | | | | | | | | | | | | |
| Flow rate: | 0.45ml/min | | | | | | | | | | | | | | | | | | | |
| Wavelength: | 280nm | | | | | | | | | | | | | | | | | | | |
| Volume: | 10 μ l | | | | | | | | | | | | | | | | | | | |

3. Result

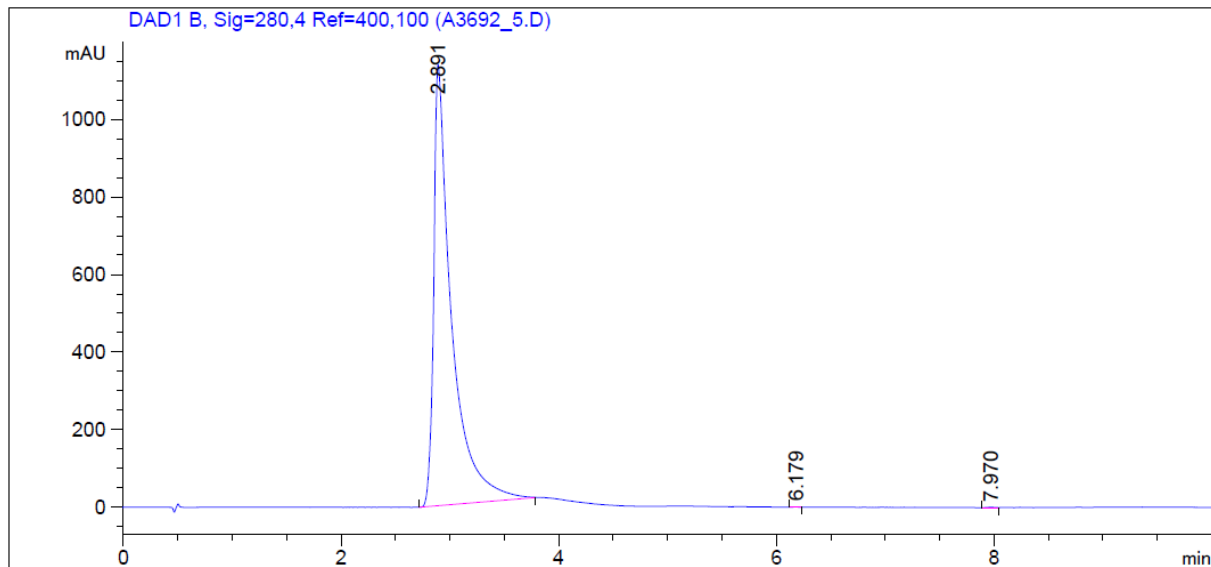

| Rank | RetTime(min) | Area(mAU*s) | Area % |
|------|--------------|-------------|---------|
| 1 | 2.891 | 1.29337e4 | 99.9309 |
| 2 | 6.179 | 3.40148 | 0.0263 |
| 3 | 7.970 | 5.54783 | 0.0429 |