

High Performance Liquid Chromatography


1. Analysis Information

Product Name:	SMIP004
Operator:	David
Injection Date:	12/12/2017 4:57:32 PM
Batch No.:	2

2. HPLC Condition

Column:	Athena C18, 3 μ m, 2.1mm \times 100 mm																
Solvent A:	0.1% H3PO4 in 100% Acetonitrile																
Solvent B:	0.1% H3PO4 in 100% Water																
Gradient:	<table border="1"> <thead> <tr> <th>Time</th> <th>A</th> <th>B</th> </tr> </thead> <tbody> <tr> <td>0.0min</td> <td>10%</td> <td>90%</td> </tr> <tr> <td>6.0min</td> <td>95%</td> <td>5%</td> </tr> <tr> <td>10.0 min</td> <td>95%</td> <td>5%</td> </tr> <tr> <td>10.0min</td> <td>Stop</td> <td>Stop</td> </tr> </tbody> </table>		Time	A	B	0.0min	10%	90%	6.0min	95%	5%	10.0 min	95%	5%	10.0min	Stop	Stop
Time	A	B															
0.0min	10%	90%															
6.0min	95%	5%															
10.0 min	95%	5%															
10.0min	Stop	Stop															
Flow rate:	0.45ml/min																
Wavelength:	210nm																
Volume:	10 μ l																

3. Result

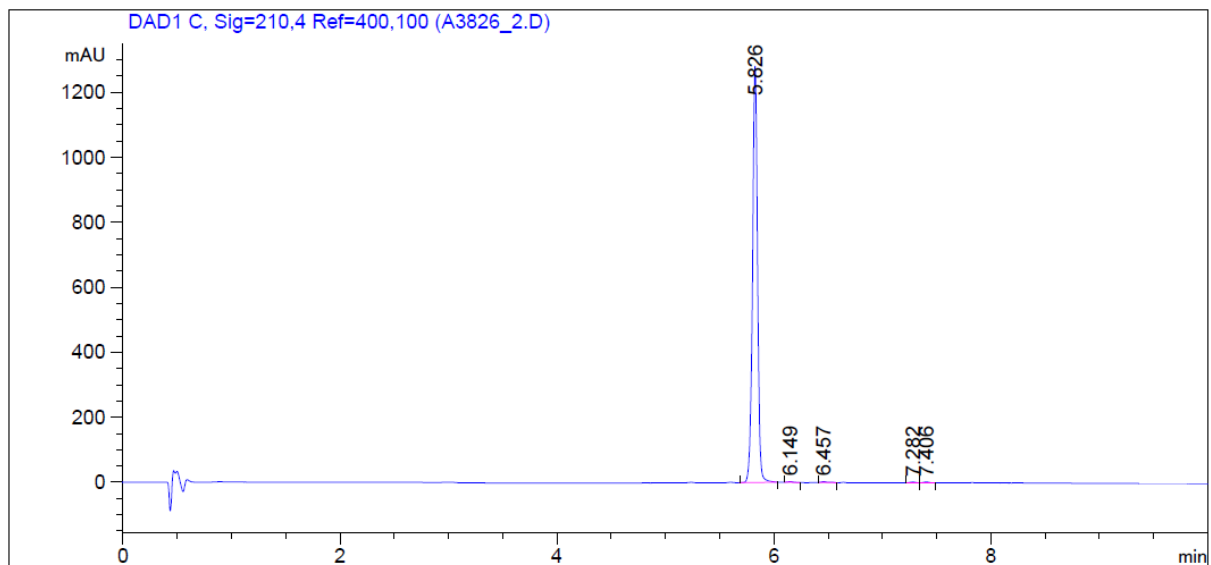

Rank	RetTime(min)	Area(mAU*s)	Area %
1	5.826	4111.57178	99.1191
2	6.149	7.09676	0.1711
3	6.457	13.22653	0.3189
4	7.282	7.67078	0.1849
5	7.406	8.54664	0.2060