

High Performance Liquid Chromatography

Analysis Information

Product Name: NLG919
Operator: David
Injection Date: 4/27/2020 8:08:07 PM
Batch No.: 2

HPLC Condition


Column : ZORBAX Eclipse Pluse C18 3.5 μ m 4.6mmx100mm
Solvent A: H2O+0.1%TFA
Solvent B: ACN+0.1%TFA

Gradient:

Time	A	B
0.0min	80%	20%
2.0min	80%	20%
7.0min	5%	95%
10.00min	0%	100%
12.00min	0%	100%
15.00min	Stop	Stop

Flow rate: 1mL/min
Wavelength: 270nm
Volume: 5 μ l

Result

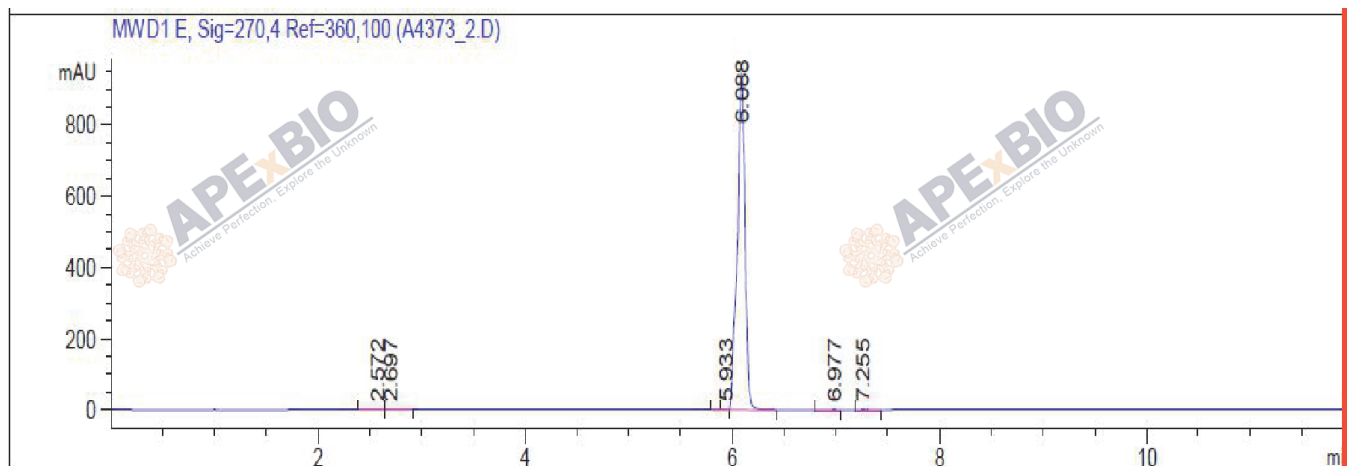

Rank	RetTime(min)	Area(mAU*s)	Area %
1	2.572	2.50854	0.0511
2	2.697	2.25602	0.0460
3	5.933	3.43556	0.0700
4	6.088	4895.43262	99.7916
5	6.977	1.00746	0.0205
6	7.255	1.01797	0.0208

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com