

# High Performance Liquid Chromatography

## Analysis Information

**Product Name:** Flurizan  
**Operator:** David  
**Injection Date:** 4/27/2020 8:41:05 PM  
**Batch No.:** 2

## HPLC Condition


**Column :** ZORBAX Eclipse Pluse C18 3.5µm 4.6mmx100mm  
**Solvent A:** H2O+0.1%TFA  
**Solvent B:** ACN+0.1%TFA

**Gradient:**

Time	A	B
0.0min	80%	20%
2.0min	80%	20%
7.0min	5%	95%
10.00min	0%	100%
12.00min	0%	100%
15.00min	Stop	Stop

**Flow rate:** 1mL/min  
**Wavelength:** 280nm  
**Volume:** 5µl

## Result

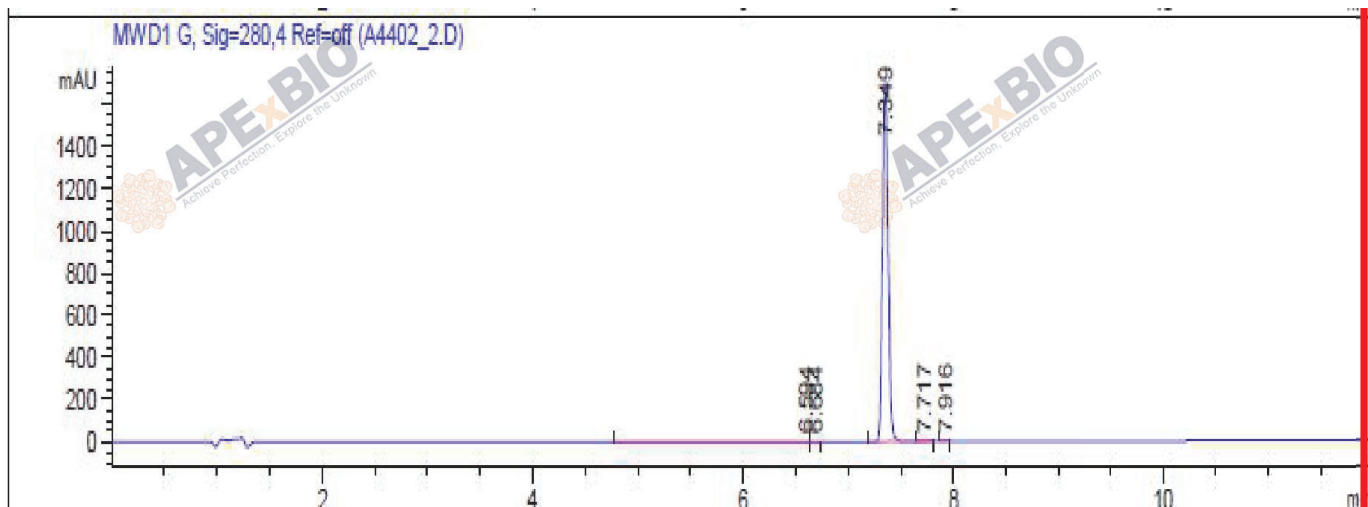

Rank	RetTime(min)	Area(mAU*s)	Area %
1	6.594	12.12569	0.1892
2	6.684	5.56370e-1	8.680e-3
3	7.349	6394.75000	99.7692
4	7.717	1.55843	0.0243
5	7.916	5.52201e-1	8.615e-3

## Caution

**FOR RESEARCH PURPOSES ONLY.**

**NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.**

**APExBIO Technology**

[www.apexbt.com](http://www.apexbt.com)

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: [info@apexbt.com](mailto:info@apexbt.com)