


## 1. Analysis Information

|                 |                       |
|-----------------|-----------------------|
| Product Name:   | 3X FLAG Peptide       |
| Operator:       | David                 |
| Injection Date: | 3/18/2013 05:04:42 PM |
| Inj. Volume:    | 1                     |
| Batch No.:      | 1                     |

## 2. Acquisition Parameter

|                     |                            |
|---------------------|----------------------------|
| Probe:              | ESI                        |
| Probe bias:         | -3.5kv                     |
| Nebulizer Gas Flow: | 1.5L/min                   |
| Detector:           | 1.0kv                      |
| DL:                 | -20.0v                     |
| T.Flow:             | 0.2ml/min                  |
| DL Temp:            | 250°C                      |
| B.conc:             | 50%H <sub>2</sub> O/50%ACN |
| Block Temp:         | 200°C                      |

## 3. Result

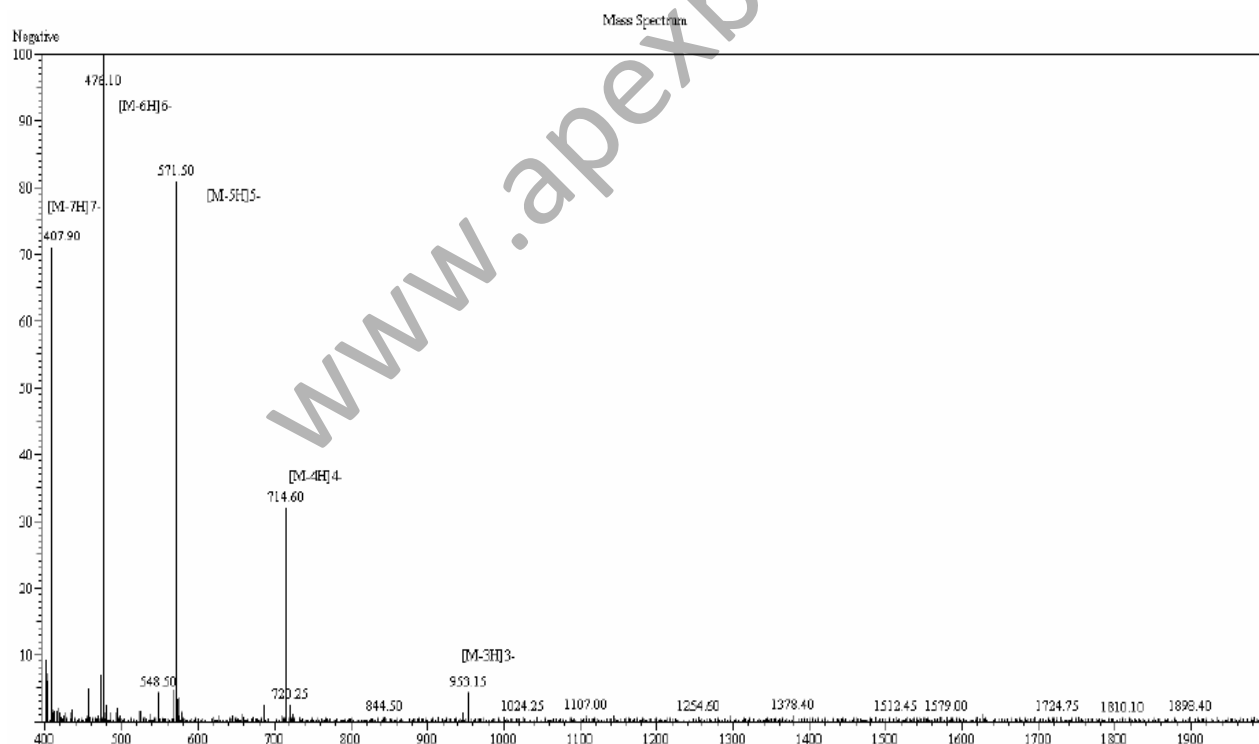

|                                       |         |
|---------------------------------------|---------|
| Molecular Weight:                     | 2861.87 |
| m/z([M-5H] <sup>5-</sup> ) Base Peak: | 571.50  |
| m/z([M-6H] <sup>6-</sup> ) Base Peak: | 476.10  |