
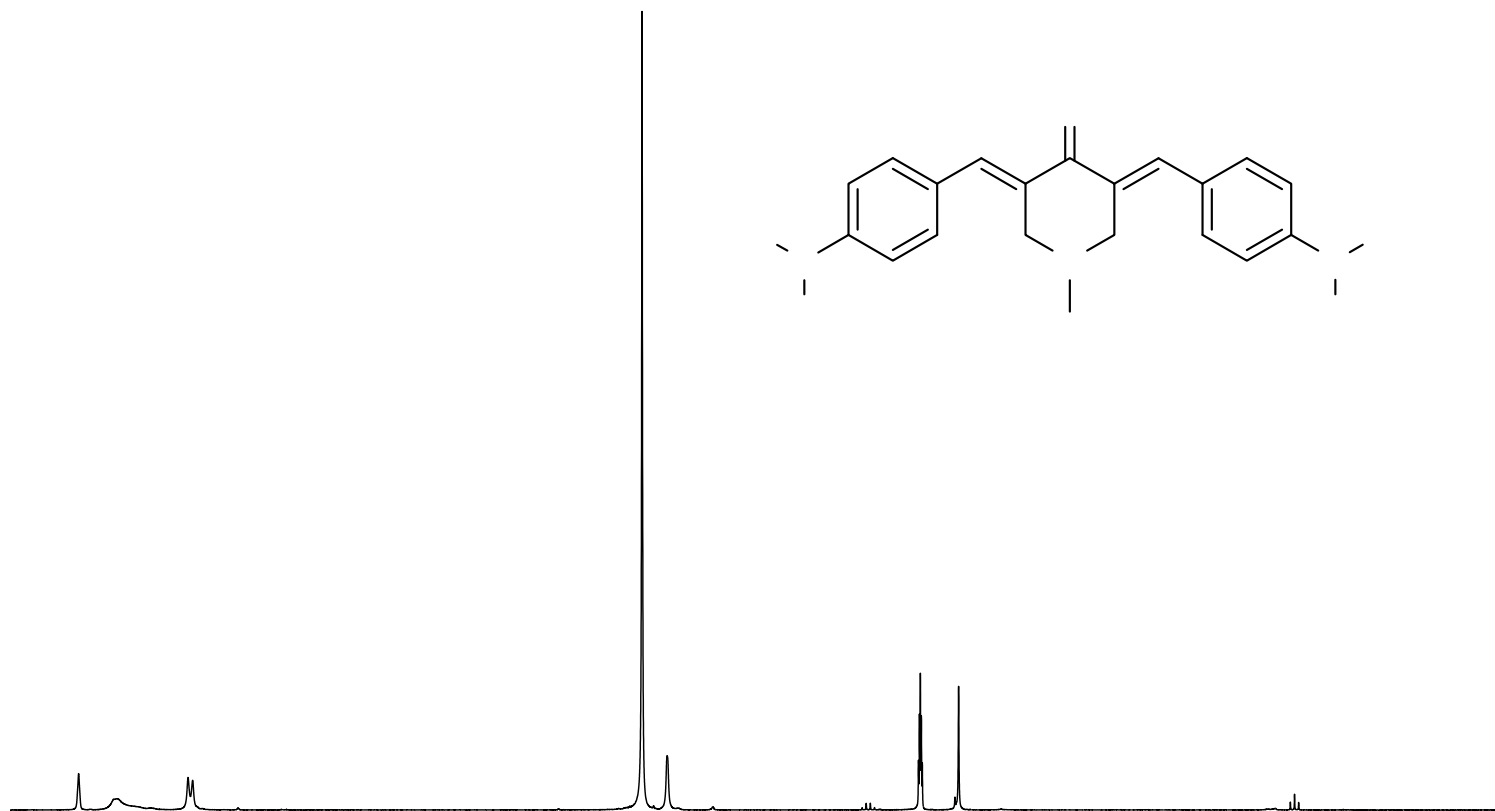


— 8.108
— 7.887
< 7.484
< 7.458

— 4.899
— 4.756

3.324
3.318
3.313
3.307
3.302
3.095

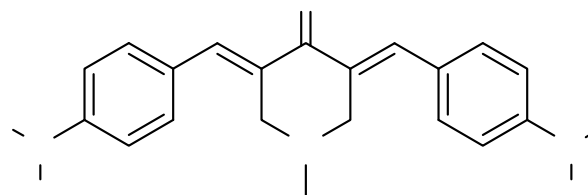

```
NAME          AM 114
EXPNO          1
PROCNO         1
Date_          20130527
Time_          9.12
INSTRUM        spect
PROBHD         5 mm PABBO BB-
PULPROG        zg30
TD             32768
SOLVENT        CD3OD_SPE
NS             8
DS             2
SWH            6009.615 Hz
FIDRES         0.183399 Hz
AQ            2.7263477 sec
RG             575
DW            83.200 usec
DE             6.50 usec
TE            298.0 K
D1            1.00000000 sec
TD0           1
```

```
===== CHANNEL f1 =====
SFO1          300.1324010 MHz
NUC1           1H
P1            12.90 usec
SI            65536
SF            300.1300052 MHz
WDW           EM
SSB           0
LB            0.30 Hz
GB           0
PC            1.00
```

1.90
4.33
4.06

3.82

3.00

8.0 7.5 7.0 6.5 6.0 5.5 5.0 4.5 4.0 3.5 3.0 2.5 2.0 1.5 1.0 ppm