



High Performance Liquid Chromatography


1. Analysis Information

Product Name:	Cyclo (-RGDFK)
Operator:	David
Injection Date:	5/06/2013 11:28:21 AM
Batch No.:	1

2. HPLC Condition

Column:	4.6*250mm,kromasil C18-5																
Solvent A:	0.1% Trifluoroacetic in 100% Acetonitrile																
Solvent B:	0.1% Trifluoroacetic in 100% Water																
Gradient:	<table border="1"> <thead> <tr> <th>Time</th> <th>A</th> <th>B</th> </tr> </thead> <tbody> <tr> <td>0.01min</td> <td>32%</td> <td>68%</td> </tr> <tr> <td>25.0min</td> <td>57%</td> <td>43%</td> </tr> <tr> <td>25.1min</td> <td>100%</td> <td>0%</td> </tr> <tr> <td>30.0min</td> <td>Stop</td> <td>Stop</td> </tr> </tbody> </table>		Time	A	B	0.01min	32%	68%	25.0min	57%	43%	25.1min	100%	0%	30.0min	Stop	Stop
Time	A	B															
0.01min	32%	68%															
25.0min	57%	43%															
25.1min	100%	0%															
30.0min	Stop	Stop															
Flow rate:	1.0ml/min																
Wavelength:	220nm																
Volume:	5µl																

3. Result

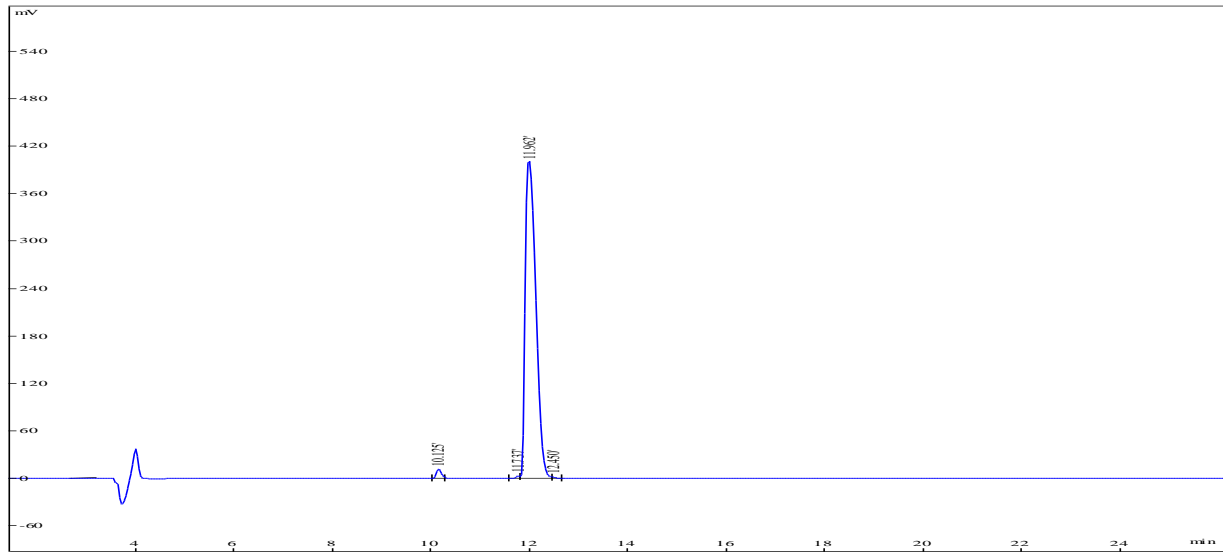

Rank	RetTime(min)	Area(mAU*s)	Area %
1	10.125	86628	1.418
2	11.737	20478	0.3352
3	11.962	5993931	98.11
4	12.45	8496	0.1391