

High Performance Liquid Chromatography


1. Analysis Information

Product Name:	Q-VD(OMe)-OPh
Operator:	David
Injection Date:	3/06/2014 14:10:16 PM
Batch No.:	2

2. HPLC Condition

Column:	xBridge C18,4.6*150mm,3.5 μ m													
Solvent A:	0.1% Trifluoroacetic in 100% Acetonitrile													
Solvent B:	0.1% Trifluoroacetic in 100% Water													
Gradient:	<table border="1"><thead><tr><th>Time</th><th>A</th><th>B</th></tr></thead><tbody><tr><td>0.0min</td><td>50%</td><td>50%</td></tr><tr><td>15.0min</td><td>100%</td><td>0%</td></tr><tr><td>15.0min</td><td>Stop</td><td>Stop</td></tr></tbody></table>		Time	A	B	0.0min	50%	50%	15.0min	100%	0%	15.0min	Stop	Stop
Time	A	B												
0.0min	50%	50%												
15.0min	100%	0%												
15.0min	Stop	Stop												
Flow rate:	0.6ml/min													
Wavelength:	254nm													
Volume:	10 μ l													

3. Result

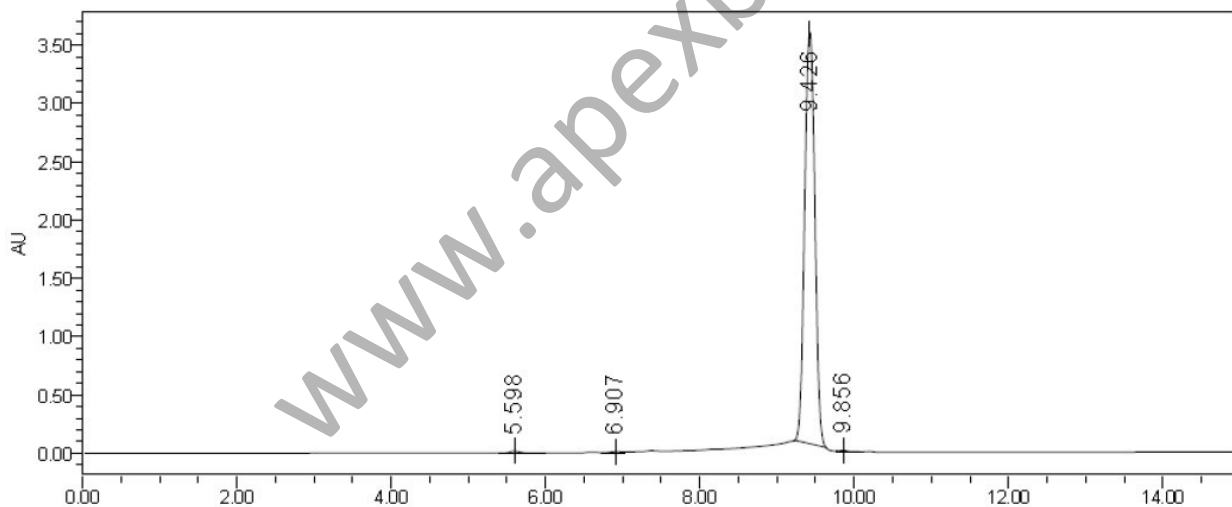

Rank	RetTime(min)	Area(mAU*s)	Area %
1	5.598	139601	0.43
2	6.907	121629	0.37
3	9.426	32268384	98.52
4	9.856	223429	0.68