


10.73

7.52
7.50
7.46
7.42
7.40
7.38
7.36
7.22
7.20
6.98
6.96
6.94
6.91
6.90
6.88
6.47
6.43

4.05
4.03
4.02
4.00
3.85

2.84
2.82
2.77
2.50
2.30
1.99
1.90
1.79
1.17
1.15
1.04
1.02
1.00

Parameter	Value
1 Title	A8178
2 Solvent	DMSO
3 Acquisition Date	2014-03-14T17:24:10
4 Modification Date	2014-03-15T14:34:10
5 Spectrometer Frequency	400.13

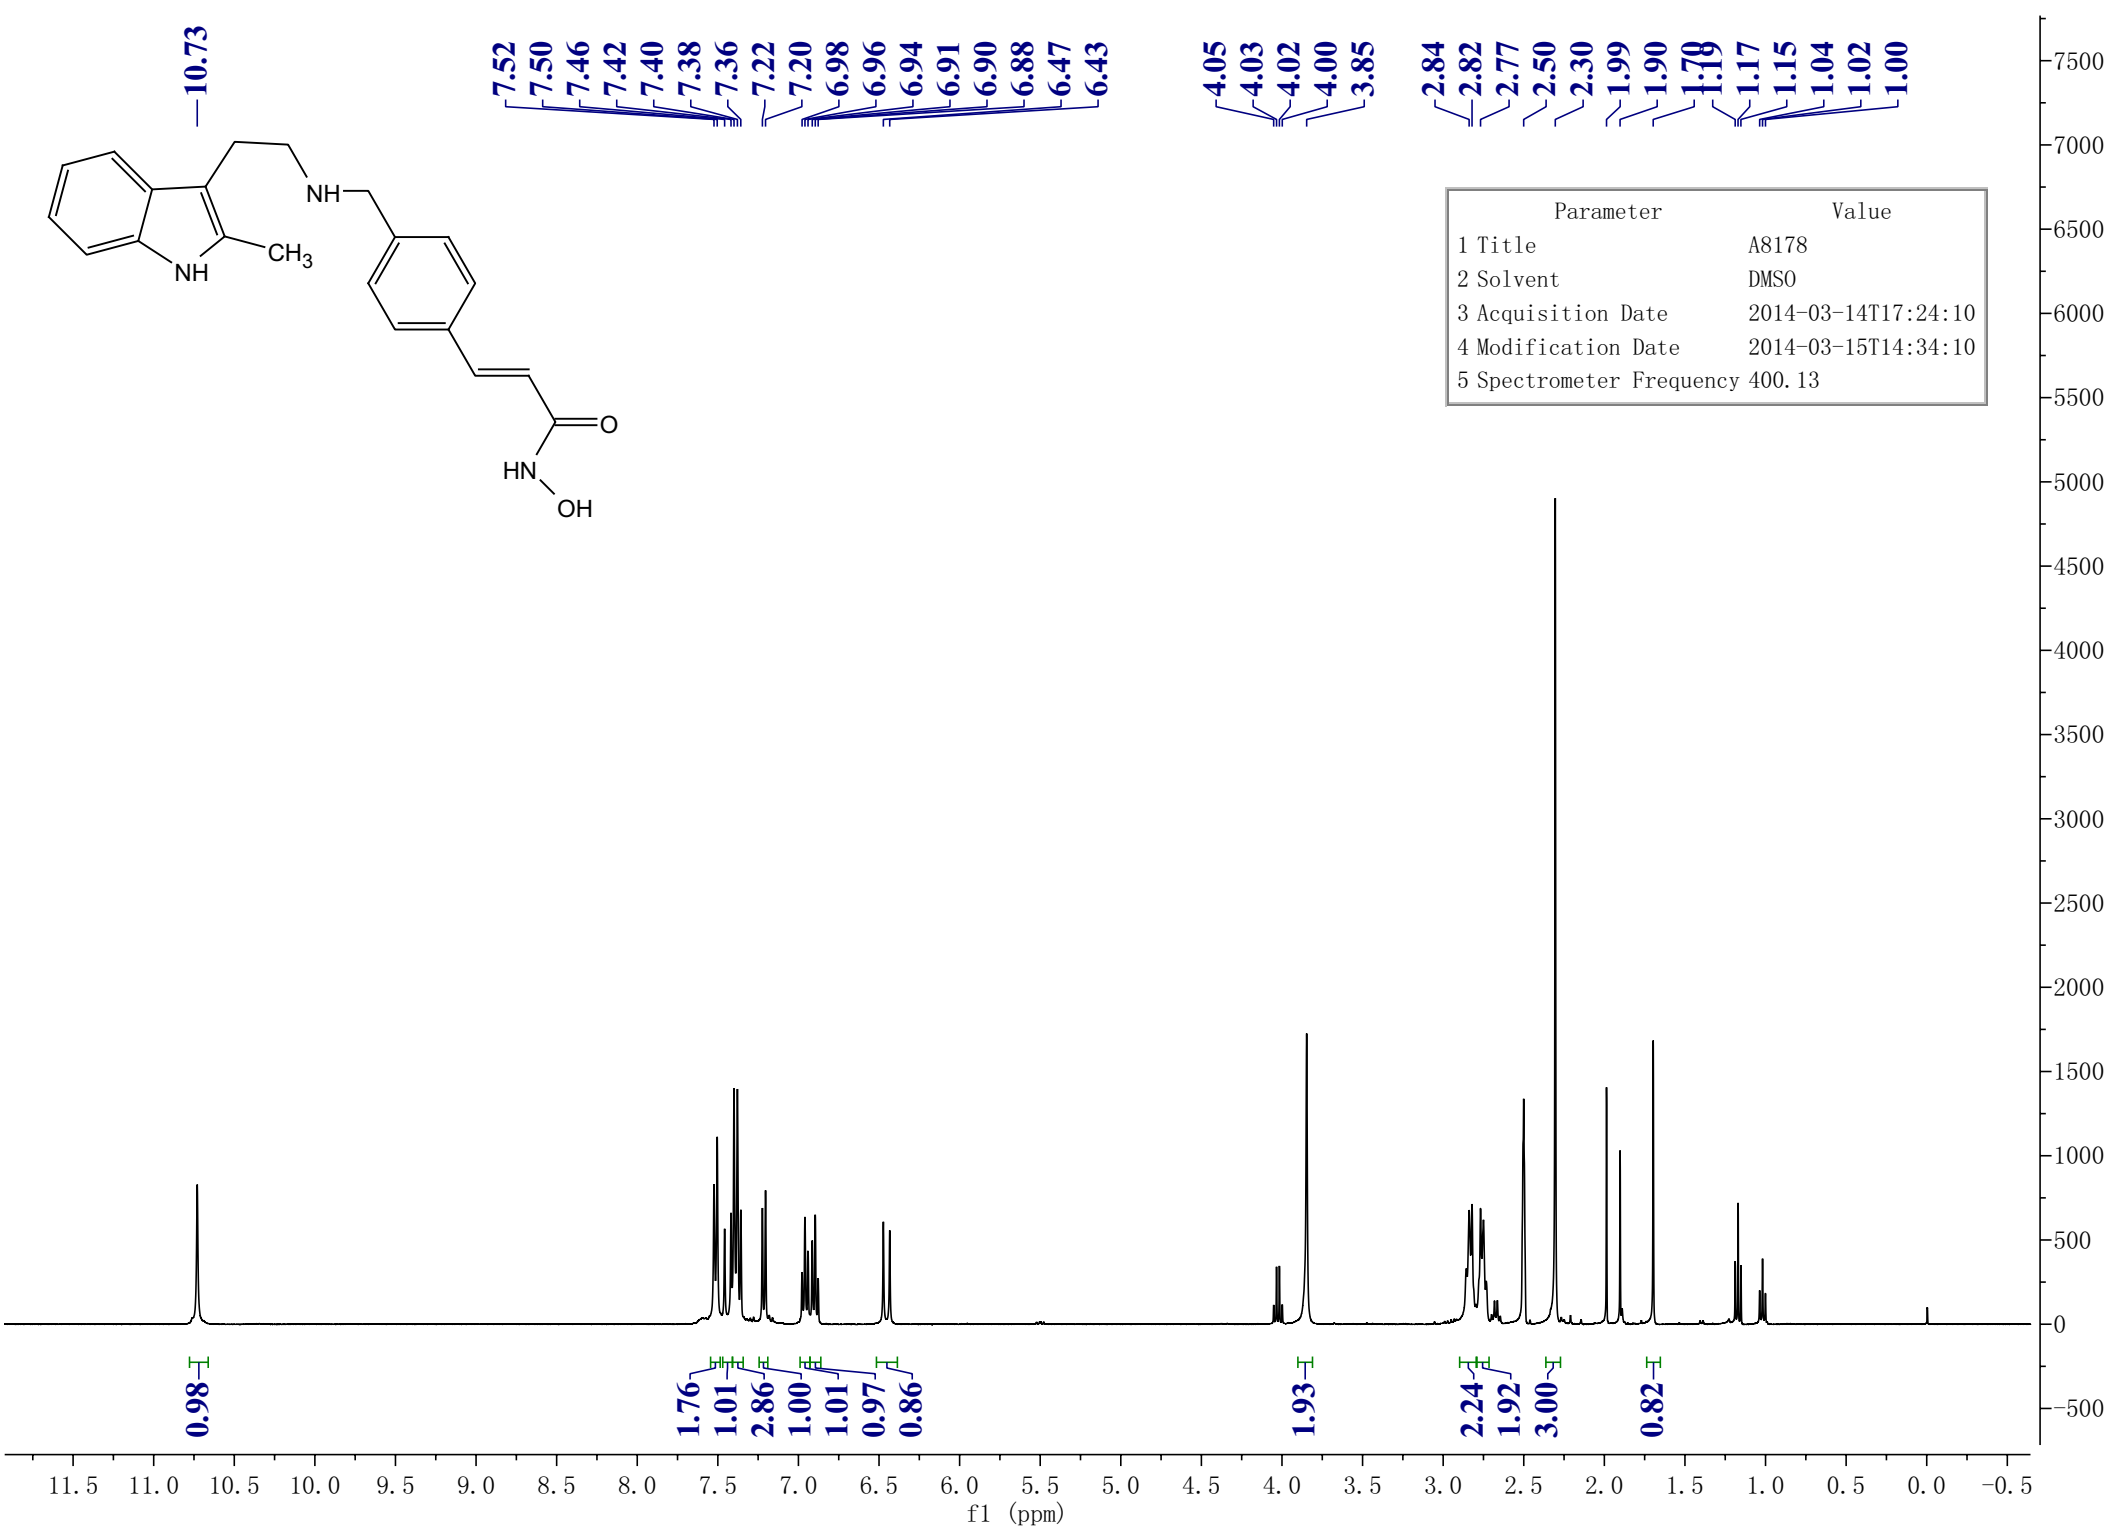

0.98

1.76
1.01
2.86
1.00
1.01
0.97
0.86

1.93

2.24
1.92
3.00

0.82