



High Performance Liquid Chromatography


1. Analysis Information

Product Name:	DAPT (GSI-IX)
Operator:	David
Injection Date:	9/28/2013 02:11:15 PM
Batch No.:	1

2. HPLC Condition

Column:	Waters XBridge C18, 3 μ m, 3 mm \times 100 mm																
Solvent A:	0.1% H ₃ PO ₄ in 100% Acetonitrile																
Solvent B:	0.1% H ₃ PO ₄ in 100% Water																
Gradient:	<table border="1"><thead><tr><th>Time</th><th>A</th><th>B</th></tr></thead><tbody><tr><td>0.0min</td><td>10%</td><td>90%</td></tr><tr><td>30.0min</td><td>70%</td><td>30%</td></tr><tr><td>35.0min</td><td>100%</td><td>0%</td></tr><tr><td>35.0min</td><td>Stop</td><td>Stop</td></tr></tbody></table>		Time	A	B	0.0min	10%	90%	30.0min	70%	30%	35.0min	100%	0%	35.0min	Stop	Stop
Time	A	B															
0.0min	10%	90%															
30.0min	70%	30%															
35.0min	100%	0%															
35.0min	Stop	Stop															
Flow rate:	1.0ml/min																
Wavelength:	220nm																
Volume:	10ul																

3. Result

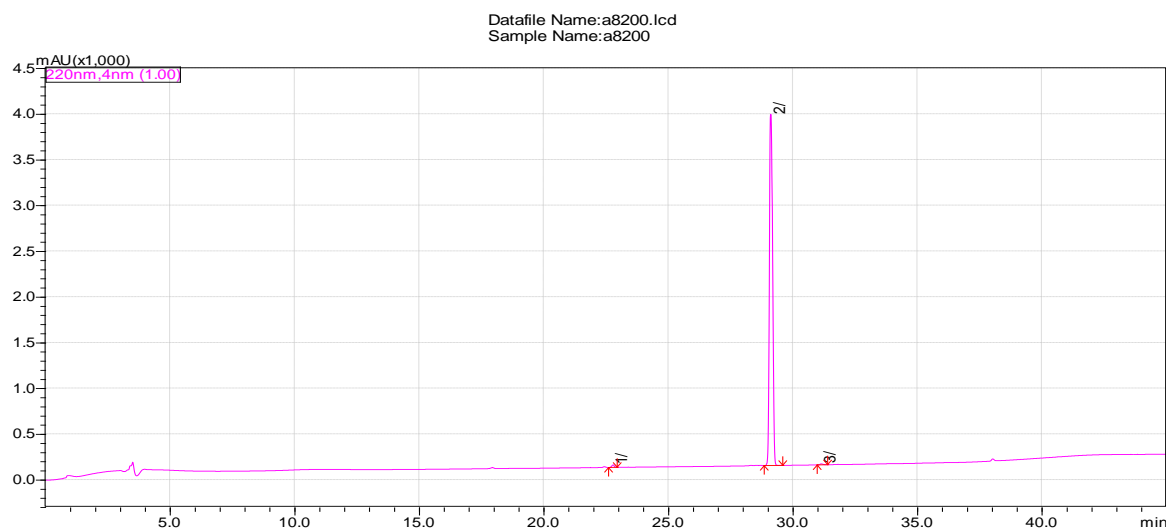

Rank	RetTime(min)	Area(mAU*s)	Area %
1	22.771	185502	0.533
2	29.103	34528956	99.186
3	31.136	97709	0.281