

## Mass Spectrometry

### Analysis Information


**Product Name:** SLIGKV-NH2  
**Operator:** David  
**Injection Date:** 2/27/2019 9:45:39 AM  
**Inj. Volume:** 1  
**Batch No.:** 2

### Acquisition Parameter

**Probe:** ESI  
**Gas Temp:** 350°C  
**Gas Flow:** 11L/min  
**Nebulizer:** 50psi  
**VCap:** 4000v  
**Fragmentor:** 70v  
**Reference:** m/z 121.050873, 922.009798  
**T.Flow:** 0.3ml/min  
**B.conc:** 20%H2O/80%ACN

# Result

Sample Name	0226	Position	P2-D7	Instrument Name	Instrument 1
User Name		Inj Vol	Unknown / Injection Program	InjPosition	
Sample Type	Sample	IRM Calibration Status	Success	Data Filename	A8677-2-POS.d
ACQ Method	20190215-HPLC-POS.m	Comment		Acquired Time	2/27/2019 9:45:39 AM (UTC+08:00)

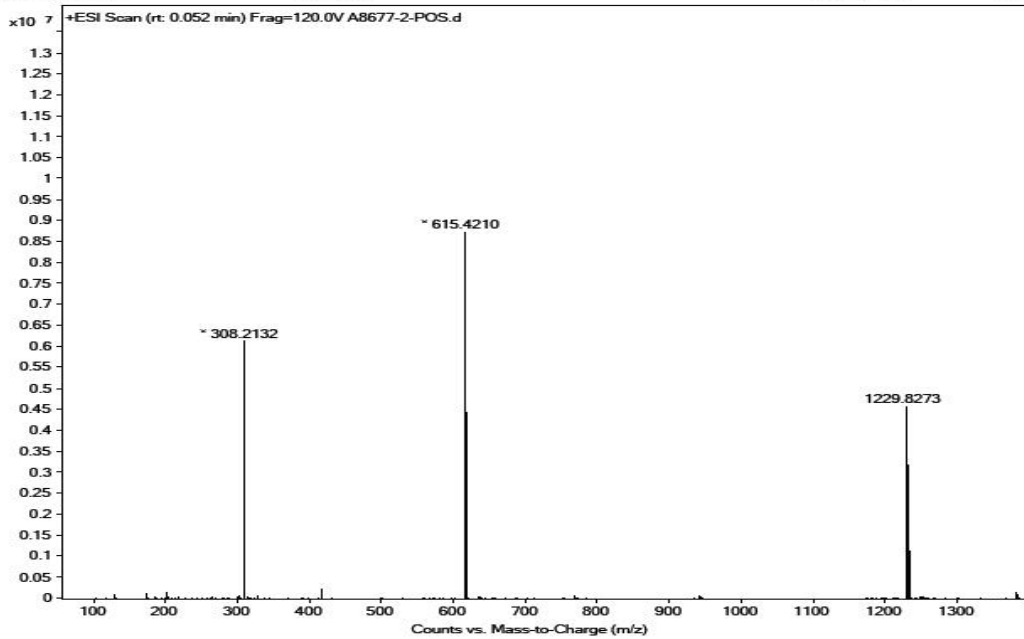

Molecular Weight: 614.78

m/z([M+H]<sup>+</sup>) Base Peak: 615.4210

m/z([M+2H]<sup>2-</sup>) Base Peak: 308.2132

## Caution

**FOR RESEARCH PURPOSES ONLY.**

**NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.**

**APExBIO Technology**

[www.apexbt.com](http://www.apexbt.com)

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: [info@apexbt.com](mailto:info@apexbt.com)