

High Performance Liquid Chromatography

Analysis Information


Product Name: AP20187
Operator: David
Injection Date: 6/30/2022 13:42:39
Batch No.: 9

HPLC Condition

Column : Agilent Eclipse Plus C18 4.6*100mm 5um
Solvent A: H2O+0.1%TFA
Solvent B: ACN+0.1%TFA
Gradient:

Time	A	B
0.0min	95%	5%
2.0min	95%	5%
4.0min	0%	100%
12.0min	0%	100%
Stop		

Flow rate: 1ml/min
Wavelength: 214nm
Volume: 5µl

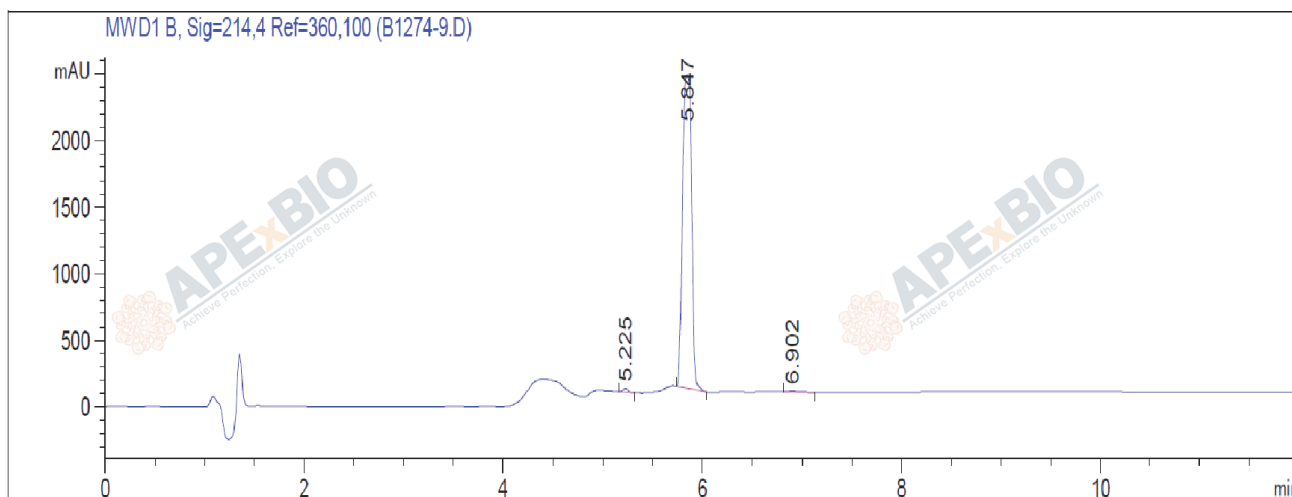

Rank	RetTime(min)	Area(mAU*s)	Area %
1	5.225	98.06385	0.6509
2	5.847	1.49011e4	98.9127
3	6.902	65.73982	0.4364

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com