

1. Analysis Information

Product Name:	AP20187
Operator:	David
Injection Date:	8/21/2017 11:26:28 AM
Inj. Volume:	1
Batch No.:	8


2. Acquisition Parameter

Probe:	ESI
Gas Temp:	350°C
Gas Flow:	11L/min
Nebulizer:	50psi
VCap:	4000v
Fragmentor:	70v
Reference:	m/z 121.050873, 922.009798
T.Flow:	0.3ml/min
B.conc:	20%H ₂ O/80%ACN

3. Result

20170821-B2-0818 3 (0.168) Cm (3:4)

1: Scan ES+
1.41e7

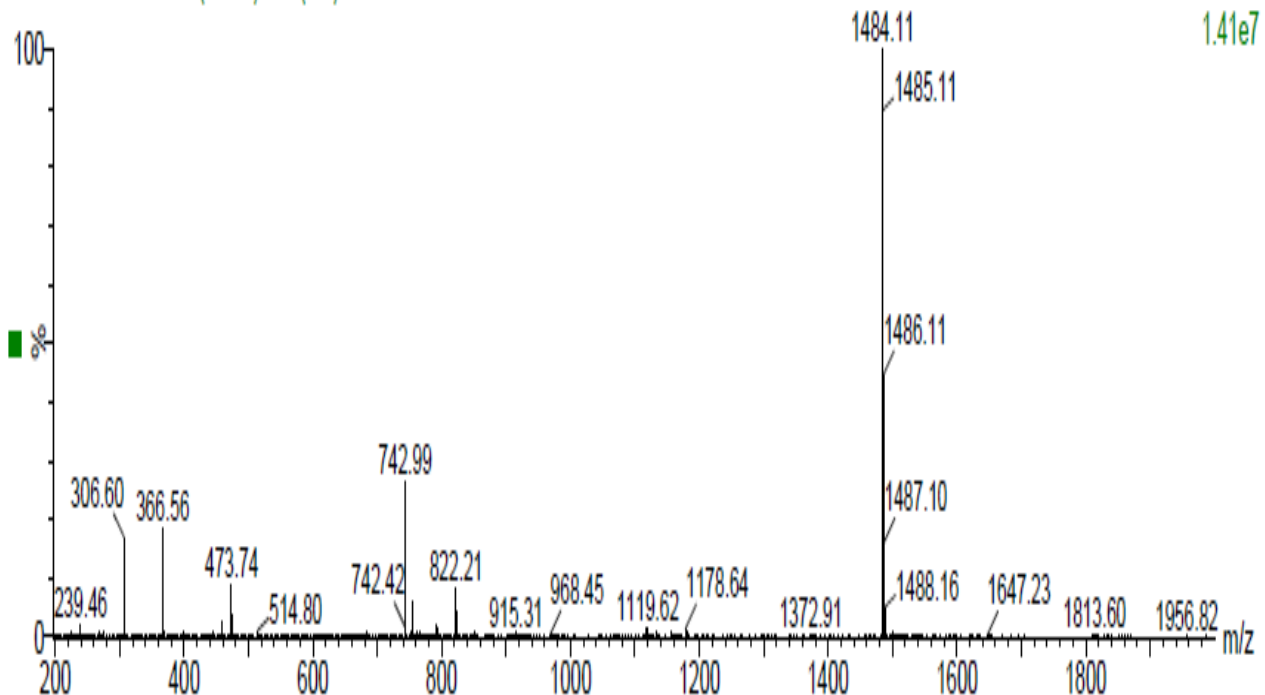

Molecular Weight:	1482.75
m/z(M+2H) Base Peak :	1484.11
m/z(M+3H) Base Peak :	1485.11