

High Performance Liquid Chromatography


1. Analysis Information

Product Name:	Pilocarpine HCl
Operator:	David
Injection Date:	5/3/2018 3:17:17 PM
Batch No.:	3

2. HPLC Condition

Column:	Athena C18, 3 μ m, 2.1mm \times 100 mm																			
Solvent A:	0.1% H ₃ PO ₄ in 100% Acetonitrile																			
Solvent B:	0.1% H ₃ PO ₄ in 100% Water																			
Gradient:	<table border="1"> <thead> <tr> <th>Time</th> <th>A</th> <th>B</th> </tr> </thead> <tbody> <tr> <td>0.0min</td> <td>0%</td> <td>100%</td> </tr> <tr> <td>2.0min</td> <td>0%</td> <td>100%</td> </tr> <tr> <td>7.0min</td> <td>95%</td> <td>5%</td> </tr> <tr> <td>10.0 min</td> <td>95%</td> <td>5%</td> </tr> <tr> <td>10.0min</td> <td>Stop</td> <td>Stop</td> </tr> </tbody> </table>		Time	A	B	0.0min	0%	100%	2.0min	0%	100%	7.0min	95%	5%	10.0 min	95%	5%	10.0min	Stop	Stop
Time	A	B																		
0.0min	0%	100%																		
2.0min	0%	100%																		
7.0min	95%	5%																		
10.0 min	95%	5%																		
10.0min	Stop	Stop																		
Flow rate:	0.45ml/min																			
Wavelength:	210nm																			
Volume:	10 μ l																			

3. Result

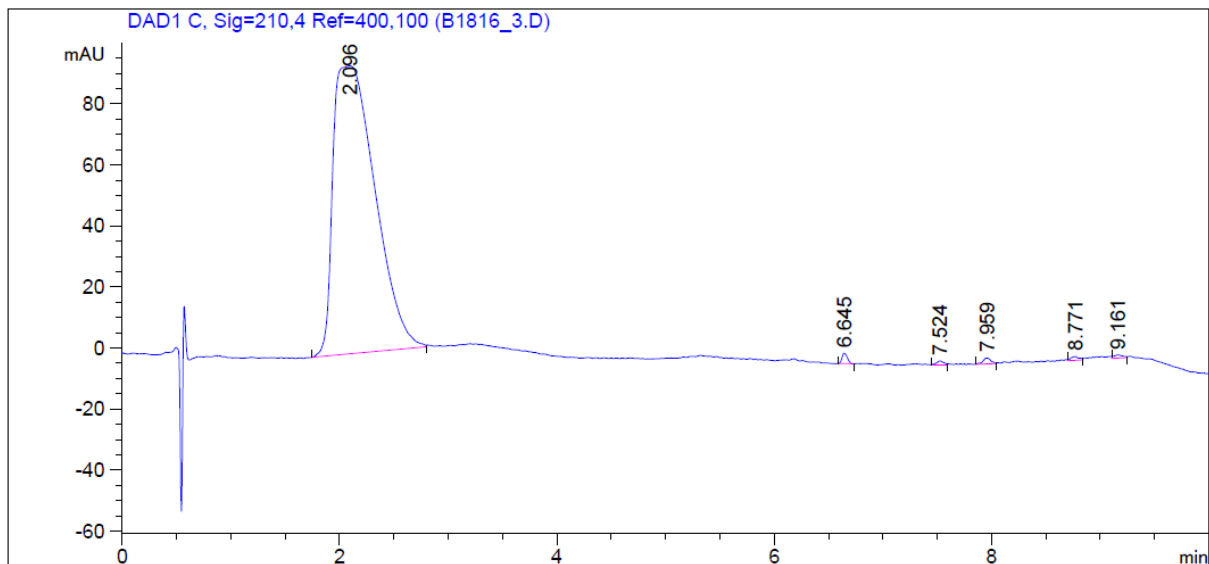

Rank	RetTime(min)	Area(mAU*s)	Area %
1	2.096	2528.85669	98.4698
2	6.645	11.72357	0.4565
3	7.524	5.37235	0.2092
4	7.959	9.82944	0.3827
5	8.771	6.42929	0.2503
6	9.161	5.94247	0.2314