

# High Performance Liquid Chromatography

## Analysis Information


**Product Name:** Diltiazem HCl  
**Operator:** David  
**Injection Date:** 10/14/2021 4:51:57 PM  
**Batch No.:** 2

## HPLC Condition

**Column :** Athena C18, 3  $\mu$ m, 2.1mm  $\times$  100 mm  
**Solvent A:** ACN+0.1%TFA  
**Solvent B:** H2O+0.1%TFA  
**Gradient:**

Time	A	B
0.0min	0%	100%
1.5min	0%	100%
6.0min	95%	5%
9.0min	95%	5%
9.0min	Stop	Stop

**Flow rate:** 0.46ml/min  
**Wavelength:** 210nm  
**Volume:** 3 $\mu$ l

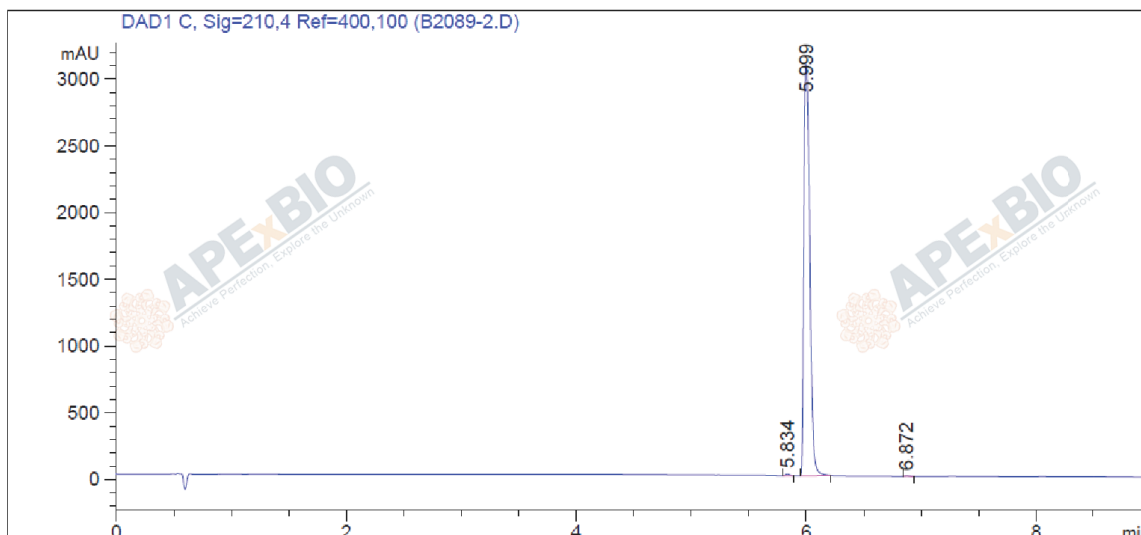

Rank	RetTime(min)	Area(mAU*s)	Area %
1	5.834	28.52163	0.2574
2	5.999	1.10466e4	99.6801
3	6.872	6.92676	0.0625

Caution

**FOR RESEARCH PURPOSES ONLY.**

**NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.**

**APEX BIO Technology**

[www.apexbt.com](http://www.apexbt.com)

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: [info@apexbt.com](mailto:info@apexbt.com)