

High Performance Liquid Chromatography

Analysis Information


Product Name: H 89 2HCl
Operator: David
Injection Date: 8/11/2021 4:59:56 PM
Batch No.: 2

HPLC Condition

Column : Athena C18, 3 μ m, 2.1mm \times 100 mm
Solvent A: ACN+0.1%TFA
Solvent B: H2O+0.1%TFA
Gradient:

| Time | A | B |
|---------|------|------|
| 0.0min | 0% | 100% |
| 1.5min | 0% | 100% |
| 6.0min | 95% | 5% |
| 9.0min | 95% | 5% |
| 25.0min | Stop | Stop |

Flow rate: 0.46ml/min
Wavelength: 210nm
Volume: 3 μ l

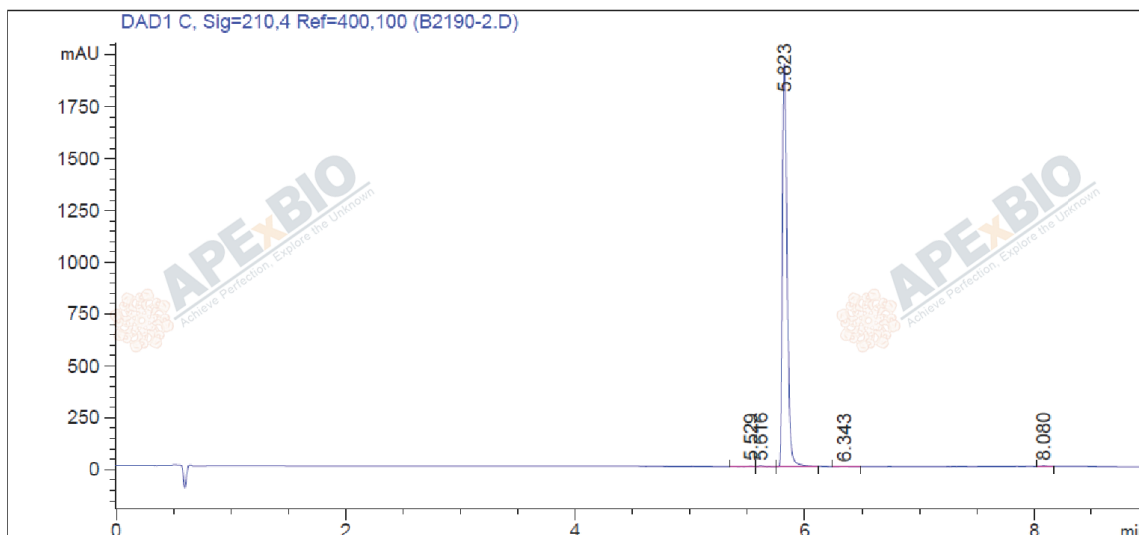

| Rank | RetTime(min) | Area(mAU*s) | Area % |
|------|--------------|-------------|---------|
| 1 | 5.529 | 9.69963 | 0.1736 |
| 2 | 5.616 | 16.41732 | 0.2938 |
| 3 | 5.823 | 5541.59131 | 99.1680 |
| 4 | 6.343 | 9.78620 | 0.1751 |
| 5 | 8.080 | 10.58938 | 0.1895 |

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com