



APEX BIO
Achieve Perfection, Explore the Unknown

High Performance Liquid Chromatography


1. Analysis Information

| | |
|-----------------|----------------------|
| Product Name: | T-5224 |
| Operator: | David |
| Injection Date: | 8/20/2015 5:16:03 PM |
| Batch No.: | 1 |

2. HPLC Condition

| Column: | Athena C18, 3 μ m, 2.1mm \times 100 mm | | | | | | | | | | | | | | | | | | | | | | |
|-------------|--|------|------|---|---|--------|-----|-----|--------|-----|----|--------|-----|----|--------|-----|-----|---------|-----|-----|---------|------|------|
| Solvent A: | 0.1% H3PO4 in 100% Acetonitrile | | | | | | | | | | | | | | | | | | | | | | |
| Solvent B: | 0.1% H3PO4 in 100% Water | | | | | | | | | | | | | | | | | | | | | | |
| Gradient: | <table border="1"> <thead> <tr> <th>Time</th> <th>A</th> <th>B</th> </tr> </thead> <tbody> <tr> <td>0.0min</td> <td>10%</td> <td>90%</td> </tr> <tr> <td>3.5min</td> <td>95%</td> <td>5%</td> </tr> <tr> <td>8.0min</td> <td>95%</td> <td>5%</td> </tr> <tr> <td>9.0min</td> <td>10%</td> <td>90%</td> </tr> <tr> <td>10.0min</td> <td>10%</td> <td>90%</td> </tr> <tr> <td>10.0min</td> <td>Stop</td> <td>Stop</td> </tr> </tbody> </table> | | Time | A | B | 0.0min | 10% | 90% | 3.5min | 95% | 5% | 8.0min | 95% | 5% | 9.0min | 10% | 90% | 10.0min | 10% | 90% | 10.0min | Stop | Stop |
| Time | A | B | | | | | | | | | | | | | | | | | | | | | |
| 0.0min | 10% | 90% | | | | | | | | | | | | | | | | | | | | | |
| 3.5min | 95% | 5% | | | | | | | | | | | | | | | | | | | | | |
| 8.0min | 95% | 5% | | | | | | | | | | | | | | | | | | | | | |
| 9.0min | 10% | 90% | | | | | | | | | | | | | | | | | | | | | |
| 10.0min | 10% | 90% | | | | | | | | | | | | | | | | | | | | | |
| 10.0min | Stop | Stop | | | | | | | | | | | | | | | | | | | | | |
| Flow rate: | 0.4ml/min | | | | | | | | | | | | | | | | | | | | | | |
| Wavelength: | 220nm | | | | | | | | | | | | | | | | | | | | | | |
| Volume: | 10 μ l | | | | | | | | | | | | | | | | | | | | | | |

3. Result

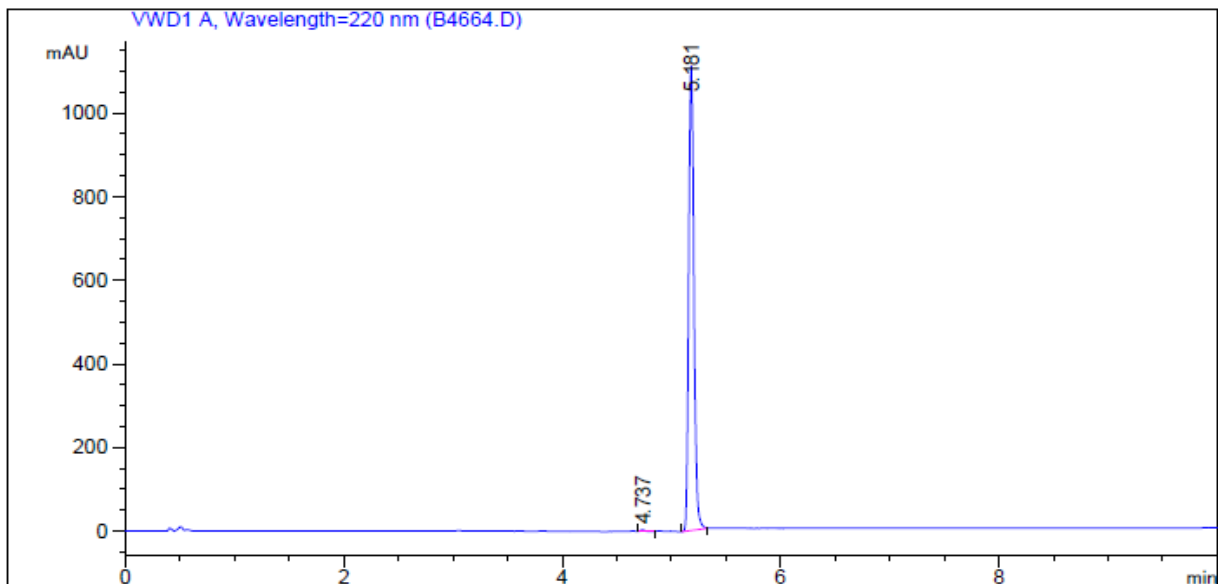

| Rank | RetTime(min) | Area(mAU*s) | Area % |
|------|--------------|-------------|---------|
| 1 | 4.737 | 11.97385 | 0.3233 |
| 2 | 5.181 | 3691.81934 | 99.6767 |