

High Performance Liquid Chromatography


1. Analysis Information

Product Name:	Verdinexor (KPT-335)
Operator:	David
Injection Date:	7/7/2015 8:55:06 AM
Batch No.:	1

2. HPLC Condition

Column:	Athena C18, 3 μ m, 2.1mm \times 100 mm																			
Solvent A:	0.1% H3PO4 in 100% Acetonitrile																			
Solvent B:	0.1% H3PO4 in 100% Water																			
Gradient:	<table border="1"><thead><tr><th>Time</th><th>A</th><th>B</th></tr></thead><tbody><tr><td>0.0min</td><td>0%</td><td>100%</td></tr><tr><td>8.0min</td><td>0%</td><td>100%</td></tr><tr><td>22.5min</td><td>95%</td><td>5%</td></tr><tr><td>30.0min</td><td>0%</td><td>100%</td></tr><tr><td>30.0min</td><td>Stop</td><td>Stop</td></tr></tbody></table>		Time	A	B	0.0min	0%	100%	8.0min	0%	100%	22.5min	95%	5%	30.0min	0%	100%	30.0min	Stop	Stop
Time	A	B																		
0.0min	0%	100%																		
8.0min	0%	100%																		
22.5min	95%	5%																		
30.0min	0%	100%																		
30.0min	Stop	Stop																		
Flow rate:	0.4ml/min																			
Wavelength:	220m																			
Volume:	10 μ l																			

3. Result

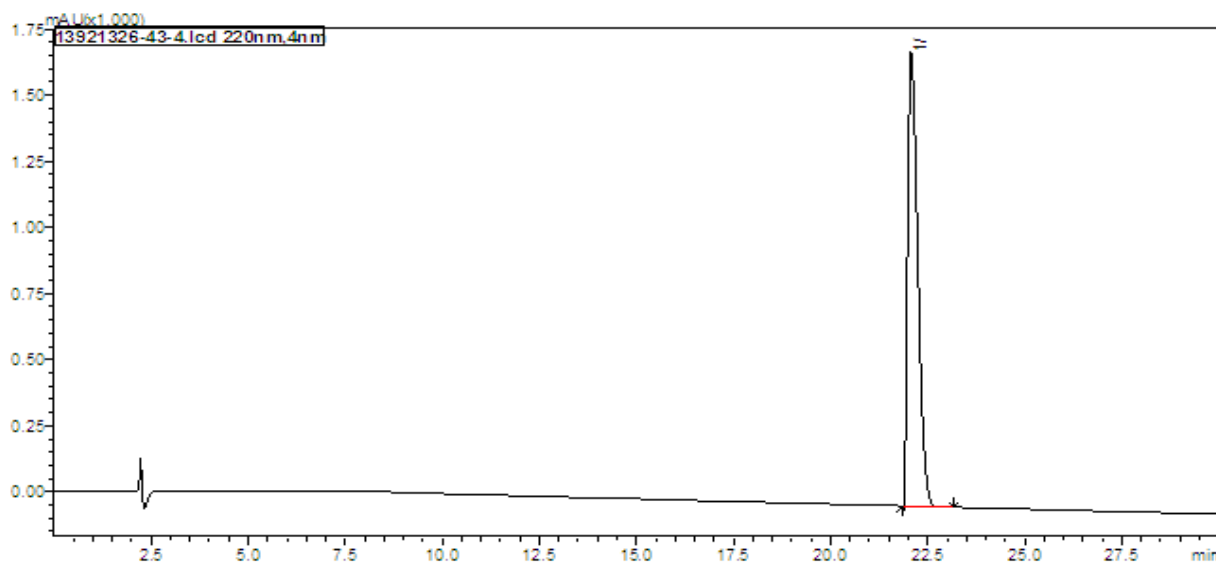

Rank	RetTime(min)	Area(mAU*s)	Area %
1	22.070	31257003	100.000