



High Performance Liquid Chromatography


1. Analysis Information

Product Name:	BLZ945
Operator:	David
Injection Date:	10/21/2016 6:23:15 PM
Batch No.:	3

2. HPLC Condition

Column:	Athena C18, 3 μ m, 2.1mm \times 100 mm																
Solvent A:	0.1% H3PO4 in 100% Acetonitrile																
Solvent B:	0.1% H3PO4 in 100% Water																
Gradient:	<table border="1"><thead><tr><th>Time</th><th>A</th><th>B</th></tr></thead><tbody><tr><td>0.0min</td><td>10%</td><td>90%</td></tr><tr><td>6.0min</td><td>95%</td><td>5%</td></tr><tr><td>10.0min</td><td>95%</td><td>5%</td></tr><tr><td>10.0min</td><td>Stop</td><td>Stop</td></tr></tbody></table>		Time	A	B	0.0min	10%	90%	6.0min	95%	5%	10.0min	95%	5%	10.0min	Stop	Stop
Time	A	B															
0.0min	10%	90%															
6.0min	95%	5%															
10.0min	95%	5%															
10.0min	Stop	Stop															
Flow rate:	0.4ml/min																
Wavelength:	230nm																
Volume:	10 μ l																

3. Result

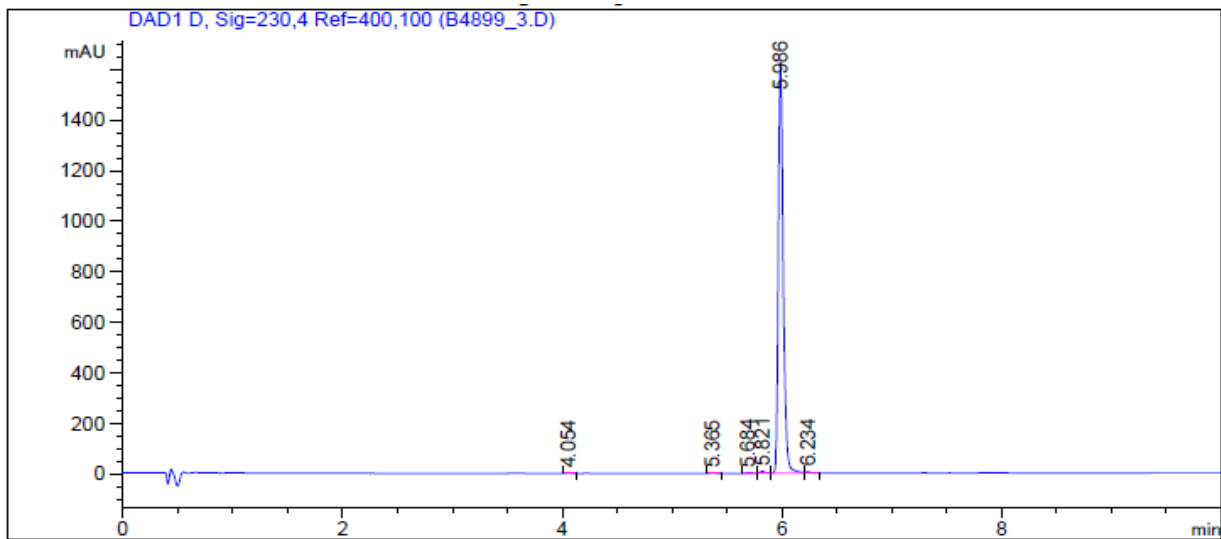

Rank	RetTime(min)	Area(mAU*s)	Area %
1	4.054	3.58530	0.0701
2	5.365	4.93629	0.0965
3	5.684	13.29580	0.2598
4	5.821	26.63071	0.5203
5	5.986	5044.99463	98.5746
6	6.234	24.50395	0.4788