

# High Performance Liquid Chromatography


## 1. Analysis Information

Product Name:	G007-LK
Operator:	David
Injection Date:	3/26/2018 5:28:47 PM
Batch No.:	4

## 2. HPLC Condition

Column:	Athena C18, 3 $\mu$ m, 2.1mm $\times$ 100 mm																			
Solvent A:	0.1% H3PO4 in 100% Acetonitrile																			
Solvent B:	0.1% H3PO4 in 100% Water																			
Gradient:	<table border="1"> <thead> <tr> <th>Time</th> <th>A</th> <th>B</th> </tr> </thead> <tbody> <tr> <td>0.0min</td> <td>0%</td> <td>100%</td> </tr> <tr> <td>2.0min</td> <td>0%</td> <td>100%</td> </tr> <tr> <td>7.0min</td> <td>95%</td> <td>5%</td> </tr> <tr> <td>10.0 min</td> <td>95%</td> <td>5%</td> </tr> <tr> <td>10.0min</td> <td>Stop</td> <td>Stop</td> </tr> </tbody> </table>		Time	A	B	0.0min	0%	100%	2.0min	0%	100%	7.0min	95%	5%	10.0 min	95%	5%	10.0min	Stop	Stop
Time	A	B																		
0.0min	0%	100%																		
2.0min	0%	100%																		
7.0min	95%	5%																		
10.0 min	95%	5%																		
10.0min	Stop	Stop																		
Flow rate:	0.45ml/min																			
Wavelength:	328nm																			
Volume:	10 $\mu$ l																			

## 3. Result

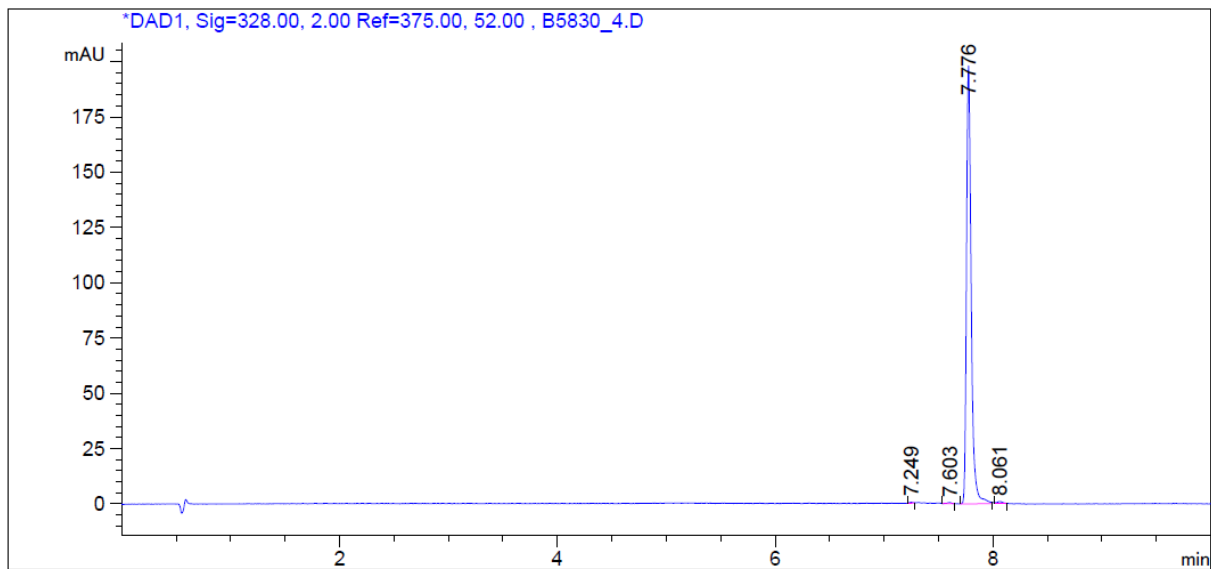

Rank	RetTime(min)	Area(mAU*s)	Area %
1	7.249	1.02408	0.1696
2	7.603	1.59195	0.2636
3	7.776	597.47809	98.9315
4	8.061	3.83674	0.6353