

1. Analysis Information

Product Name:	SCH772984 HCl
Operator:	David
Injection Date:	7/12/2018 1:51:13 PM
Inj. Volume:	1
Batch No.:	2


2. Acquisition Parameter

Probe:	ESI
Gas Temp:	350°C
Gas Flow:	11L/min
Nebulizer:	50psi
VCap:	4000v
Fragmentor:	70v
Reference:	m/z 121.050873, 922.009798
T.Flow:	0.3ml/min
B.conc:	20%H ₂ O/80%ACN

3. Result

20180712-5866-F 9 (0.156)

2: Scan ES-
2.95e6

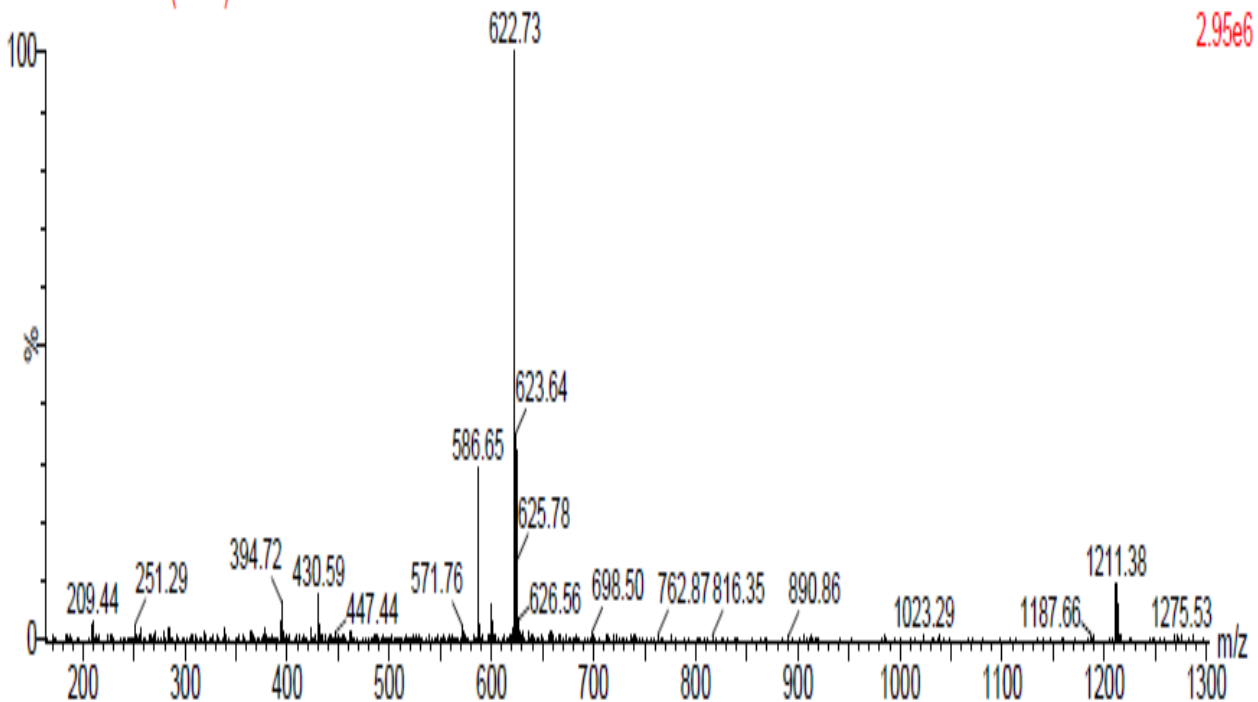

Molecular Weight:	624.17
m/z(M-2H)Base Peak :	622.73
m/z(M- H)Base Peak :	623.64