



# High Performance Liquid Chromatography


## 1. Analysis Information

Product Name:	CL-387785 (EKI-785)
Operator:	David
Injection Date:	12/27/2016 9:43:02 PM
Batch No.:	2

## 2. HPLC Condition

Column:	Athena C18, 3 $\mu$ m, 2.1mm $\times$ 100 mm																
Solvent A:	0.1% H3PO4 in 100% Acetonitrile																
Solvent B:	0.1% H3PO4 in 100% Water																
Gradient:	<table border="1"><thead><tr><th>Time</th><th>A</th><th>B</th></tr></thead><tbody><tr><td>0.0min</td><td>5%</td><td>95%</td></tr><tr><td>9.0min</td><td>95%</td><td>5%</td></tr><tr><td>15.0min</td><td>95%</td><td>5%</td></tr><tr><td>15.0min</td><td>Stop</td><td>Stop</td></tr></tbody></table>		Time	A	B	0.0min	5%	95%	9.0min	95%	5%	15.0min	95%	5%	15.0min	Stop	Stop
Time	A	B															
0.0min	5%	95%															
9.0min	95%	5%															
15.0min	95%	5%															
15.0min	Stop	Stop															
Flow rate:	0.4ml/min																
Wavelength:	254nm																
Volume:	10 $\mu$ l																

## 3. Result

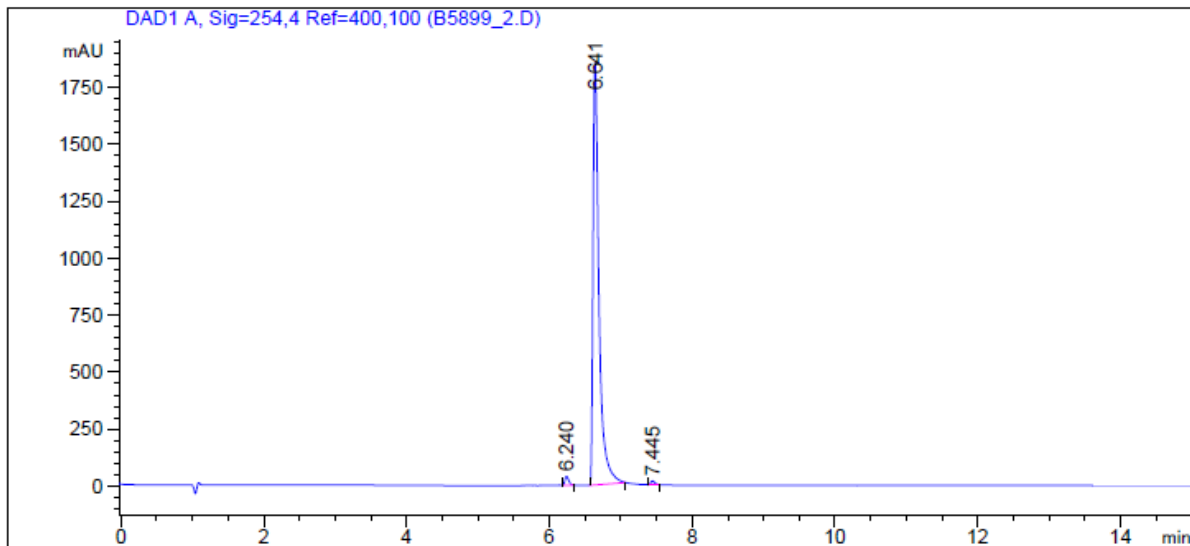

Rank	RetTime(min)	Area(mAU*s)	Area %
1	6.240	143.49745	1.3089
2	6.641	1.07535e4	98.0864
3	7.445	66.29277	0.6047