

1. Analysis Information

Product Name:	Nitrocefin
Operator:	David
Injection Date:	1/9/2017 01:22:18 PM
Inj. Volume:	1
Batch No.:	2


2. Acquisition Parameter

Probe:	ESI
Gas Temp:	350°C
Gas Flow:	11L/min
Nebulizer:	50psi
VCap:	4000v
Fragmentor:	70v
Reference:	m/z 121.050873, 922.009798
T.Flow:	0.3ml/min
B.conc:	20% H ₂ O/80% ACN

3. Result

20170109-41906-86-9-F 10 (0.174)

2: Scan ES-
2.43e7

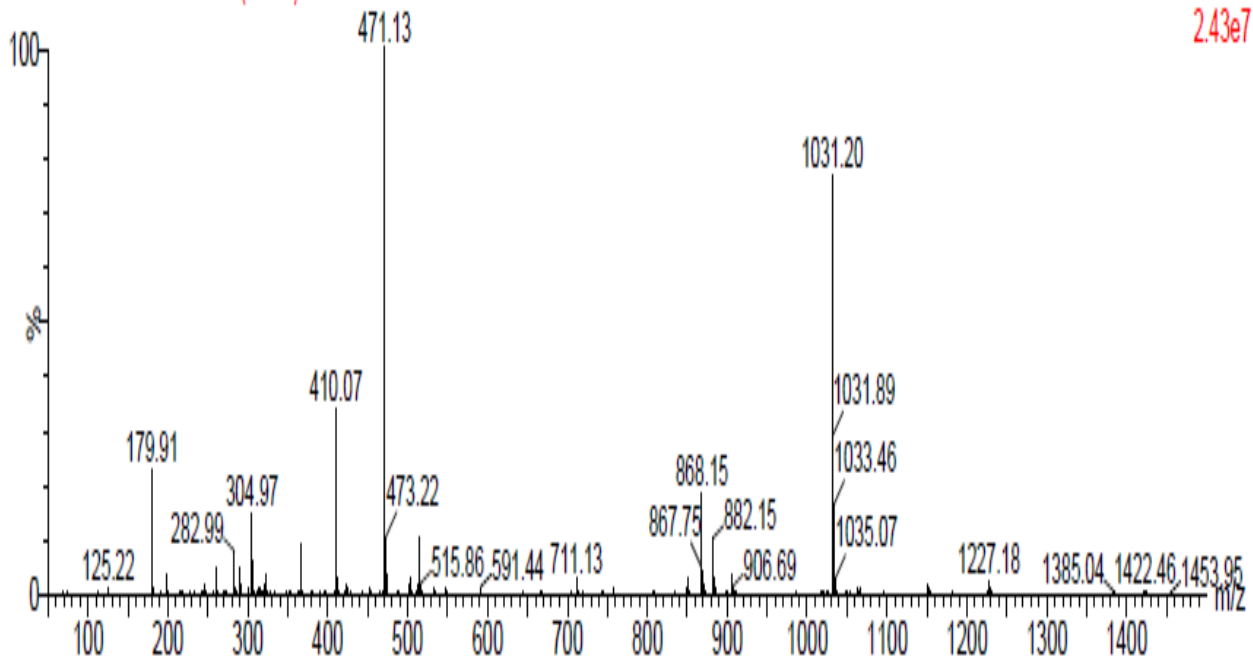

Molecular Weight:	516.50
m/z(M-2H) Base Peak :	514.86
m/z(M-H) Base Peak :	515.86