

High Performance Liquid Chromatography

1. Analysis Information

Product Name:	1400W dihydrochloride
Operator:	David
Injection Date:	2/8/2017 3:38:14 PM
Batch No.:	2


2. HPLC Condition

Column:	Athena C18, 3 μ m, 2.1mm \times 100 mm
Solvent A:	0.1% H ₃ PO ₄ in 100% Acetonitrile
Solvent B:	0.1% H ₃ PO ₄ in 100% Water

Gradient:			
	Time	A	B
	0.0min	5%	95%
	9.0min	95%	5%
	15.0min	95%	5%
	15.0min	Stop	Stop

Flow rate:	0.4ml/min
Wavelength:	210nm
Volume:	10 μ l

3. Result

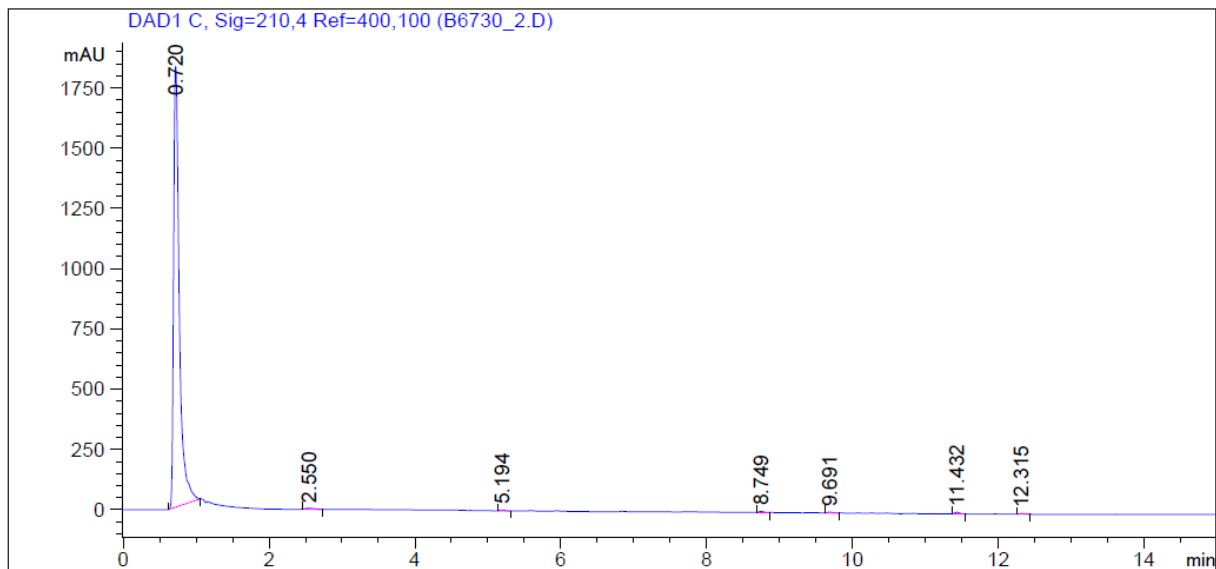

Rank	RetTime(min)	Area(mAU*s)	Area %
1	0.720	9967.47559	98.7700
2	2.550	34.26347	0.3395
3	5.194	13.36662	0.1325
4	8.749	18.12693	0.1796
5	9.691	16.11339	0.1597
6	11.432	30.87855	0.3060
7	12.315	11.37695	0.1127