

High Performance Liquid Chromatography

1. Analysis Information

Product Name:	MTT
Operator:	David
Injection Date:	7/27/2018 11:20:24 AM
Batch No.:	3


2. HPLC Condition

Column:	Boston uni-C18 5 μ m 4.6mmx250mm
Solvent A:	H2O+1% TFA
Solvent B:	ACN+1% TFA

Gradient:	Time	A	B
	0.0min	80%	20%
	2.0min	80%	20%
	7.0min	5%	95%
	10.0 min	0%	100%
	12.0 min	0%	100%
	12.10min	80%	20%
	20.0min	Stop	Stop

Flow rate:	0.25ml/min
Wavelength:	267nm
Volume:	3 μ l

3. Result

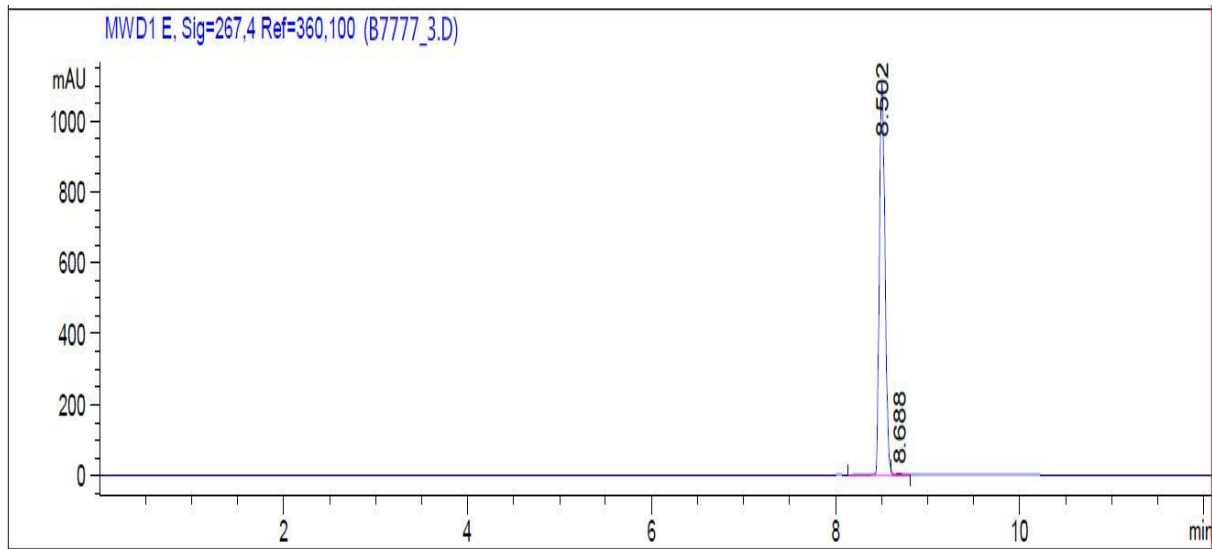

Rank	RetTime(min)	Area(mAU*s)	Area %
1	8.502	4696.15479	99.5825
2	8.688	19.68698	0.4175