


1. Analysis Information

Product Name:	BKT140
Operator:	David
Injection Date:	5/7/2018 4:39:51 PM
Inj. Volume:	1
Batch No.:	2

2. Acquisition Parameter

Probe:	ESI
Gas Temp:	350°C
Gas Flow:	11L/min
Nebulizer:	50psi
VCap:	4000v
Fragmentor:	70v
Reference:	m/z 121.050873, 922.009798
T.Flow:	0.3ml/min
B.conc:	20% H ₂ O/80% ACN

3. Result

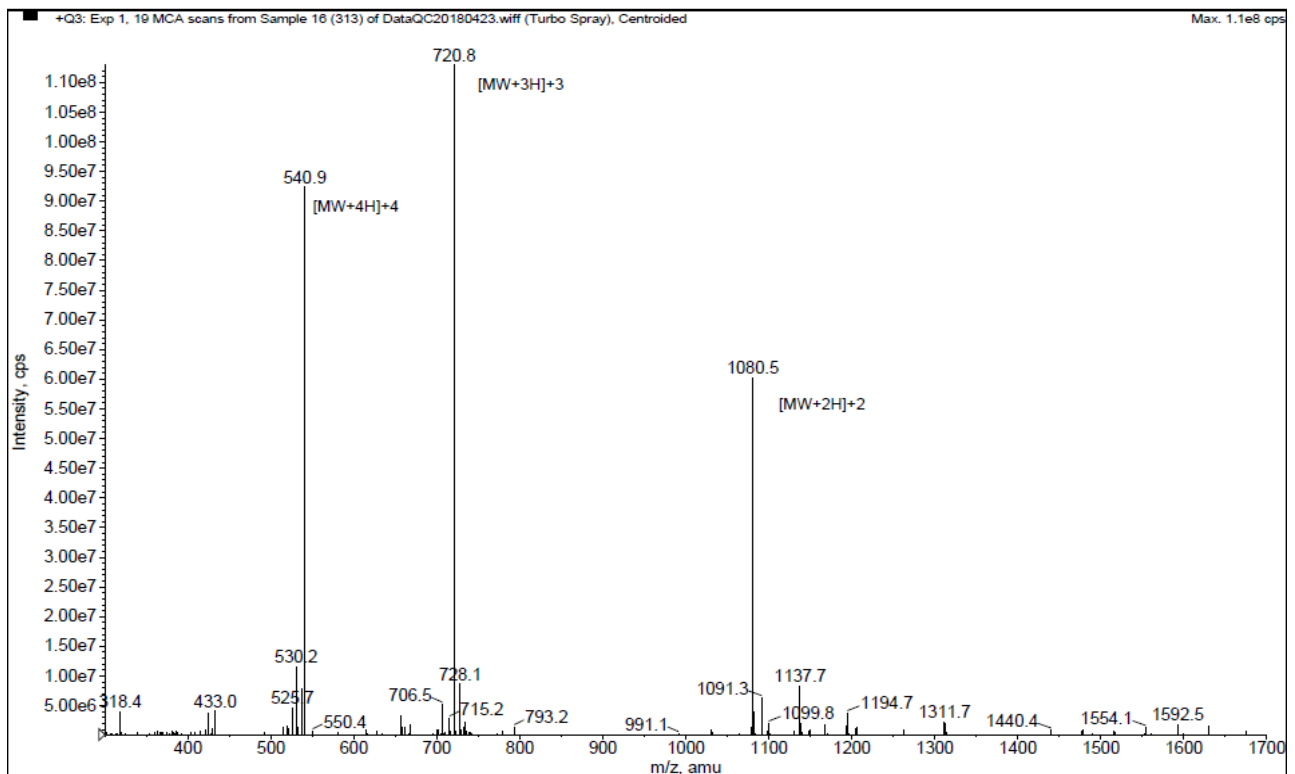

Molecular Weight:	2159.52
m/z([M+4H] ⁴⁺) Base Peak :	540.9
m/z([M+3H] ³⁺) Base Peak :	720.8
m/z([M+2H] ²⁺) Base Peak :	1080.5