

1. Analysis Information

Product Name:	CCT245737
Operator:	David
Injection Date:	6/19/2018 2:06:33 PM
Inj. Volume:	1
Batch No.:	2

2. Acquisition Parameter


Probe:	ESI
Gas Temp:	350°C
Gas Flow:	11L/min
Nebulizer:	50psi
VCap:	4000v
Fragmentor:	70v
Reference:	m/z 121.050873, 922.009798
T.Flow:	0.3ml/min
B.conc:	20%H ₂ O/80%ACN

3. Result

NT-S20180619-020

20180619-1489389-18-5-F 13 (0.217)

1: Scan ES+
7.19e7

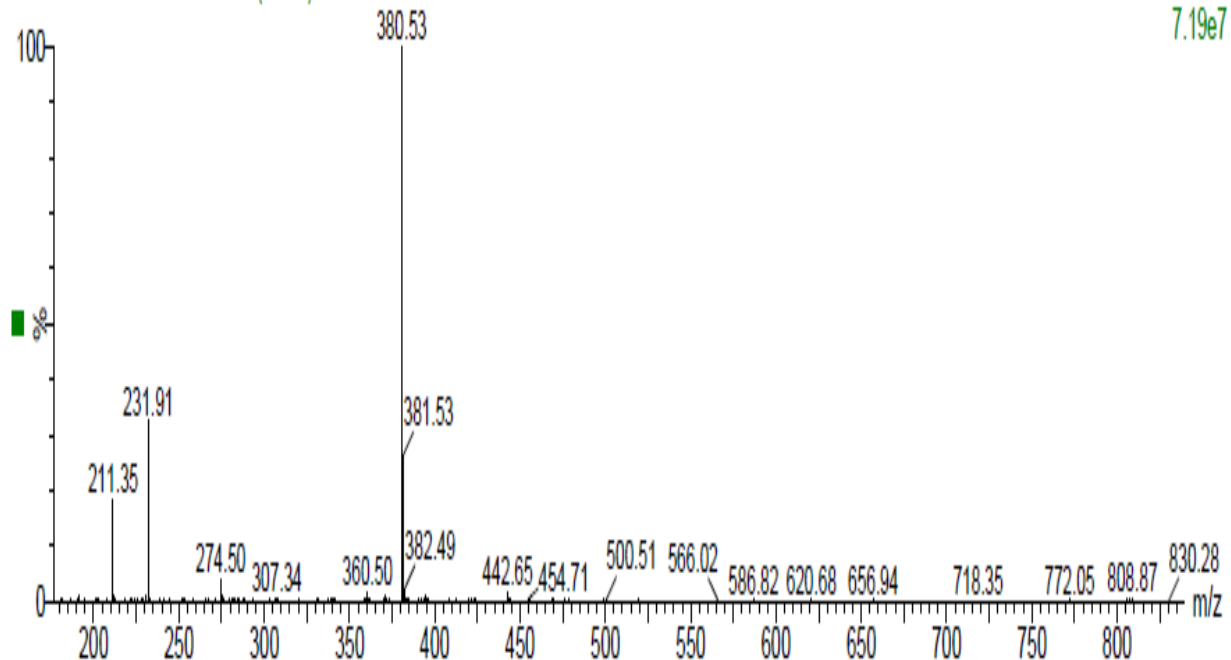

Molecular Weight:	379.34
m/z(M+H) Base Peak :	380.53