



APEX BIO
Achieve Perfection, Explore the Unknown

High Performance Liquid Chromatography


1. Analysis Information

| | |
|-----------------|----------------------|
| Product Name: | Fulvestrant |
| Operator: | David |
| Injection Date: | 6/13/2016 2:18:25 PM |
| Batch No.: | 1 |

2. HPLC Condition

| Column: | Athena C18, 3 μ m, 2.1mm \times 100 mm | | | | | | | | | | | | | | | | |
|-------------|--|------|------|---|---|--------|-----|-----|--------|-----|----|---------|-----|----|---------|------|------|
| Solvent A: | 0.1% H3PO4 in 100% Acetonitrile | | | | | | | | | | | | | | | | |
| Solvent B: | 0.1% H3PO4 in 100% Water | | | | | | | | | | | | | | | | |
| Gradient: | <table border="1"> <thead> <tr> <th>Time</th> <th>A</th> <th>B</th> </tr> </thead> <tbody> <tr> <td>0.0min</td> <td>10%</td> <td>90%</td> </tr> <tr> <td>6.0min</td> <td>95%</td> <td>5%</td> </tr> <tr> <td>10.0min</td> <td>95%</td> <td>5%</td> </tr> <tr> <td>10.0min</td> <td>Stop</td> <td>Stop</td> </tr> </tbody> </table> | | Time | A | B | 0.0min | 10% | 90% | 6.0min | 95% | 5% | 10.0min | 95% | 5% | 10.0min | Stop | Stop |
| Time | A | B | | | | | | | | | | | | | | | |
| 0.0min | 10% | 90% | | | | | | | | | | | | | | | |
| 6.0min | 95% | 5% | | | | | | | | | | | | | | | |
| 10.0min | 95% | 5% | | | | | | | | | | | | | | | |
| 10.0min | Stop | Stop | | | | | | | | | | | | | | | |
| Flow rate: | 0.4ml/min | | | | | | | | | | | | | | | | |
| Wavelength: | 210nm | | | | | | | | | | | | | | | | |
| Volume: | 10 μ l | | | | | | | | | | | | | | | | |

3. Result

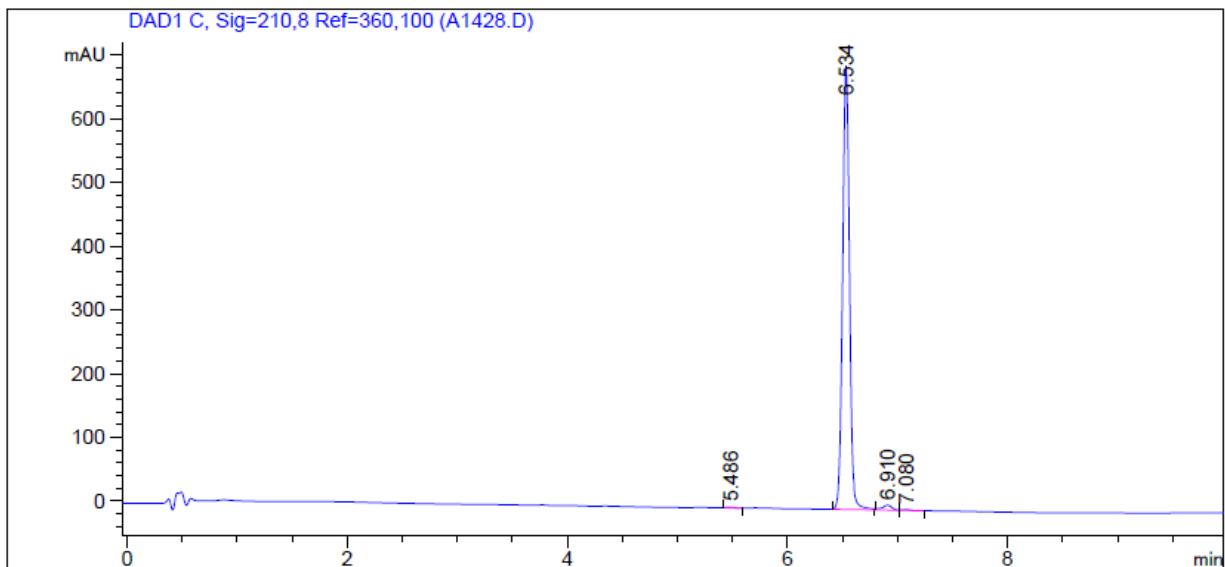

| Rank | RetTime(min) | Area(mAU*s) | Area % |
|------|--------------|-------------|---------|
| 1 | 5.486 | 4.54322 | 0.1479 |
| 2 | 6.534 | 3014.19653 | 98.0950 |
| 3 | 6.910 | 48.27014 | 1.5709 |
| 4 | 7.080 | 5.72161 | 0.1862 |