

# High Performance Liquid Chromatography

## 1. Analysis Information

Product Name:	Z-VEID-FMK
Operator:	David
Injection Date:	6/9/2017 10:06:28 AM
Batch No.:	2


## 2. HPLC Condition

Column:	Athena C18, 3 $\mu$ m, 2.1mm $\times$ 100 mm
Solvent A:	0.1% H <sub>3</sub> PO <sub>4</sub> in 100% Acetonitrile
Solvent B:	0.1% H <sub>3</sub> PO <sub>4</sub> in 100% Water

Gradient:	Time	A	B
	0.0min	0%	100%
	2.0min	0%	100%
	7.0min	95%	5%
	10.0min	95%	5%
	10.0min	Stop	Stop

Flow rate:	0.45ml/min
Wavelength:	210nm
Volume:	10 $\mu$ l

## 3. Result

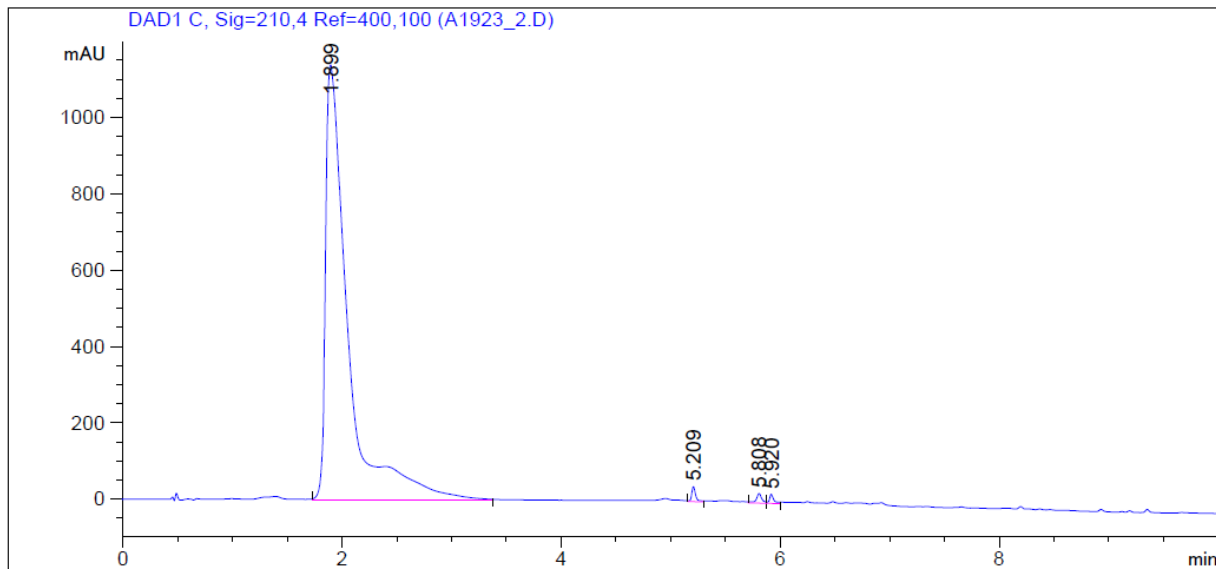

Rank	RetTime(min)	Area(mAU*s)	Area %
1	1.899	1.61394e4	98.4178
2	5.209	101.32435	0.6179
3	5.808	89.69672	0.5470
4	5.920	68.44605	0.4174