

# High Performance Liquid Chromatography


## 1. Analysis Information

Product Name:	Z-VEID-FMK
Operator:	David
Injection Date:	5/3/2013 09:15:18 AM
Batch No.:	1

## 2. HPLC Condition

Column:	Dikmal Platisil ODS,4.6*150mm,5µm,100A																
Solvent A:	100% Water																
Solvent B:	100% Acetonitrile																
Gradient:	<table border="1"> <thead> <tr> <th>Time</th> <th>A</th> <th>B</th> </tr> </thead> <tbody> <tr> <td>0.0min</td> <td>50%</td> <td>50%</td> </tr> <tr> <td>20.0min</td> <td>50%</td> <td>50%</td> </tr> <tr> <td>20.0min</td> <td>Stop</td> <td>Stop</td> </tr> <tr> <td>1.0ml/min</td> <td></td> <td></td> </tr> </tbody> </table>		Time	A	B	0.0min	50%	50%	20.0min	50%	50%	20.0min	Stop	Stop	1.0ml/min		
Time	A	B															
0.0min	50%	50%															
20.0min	50%	50%															
20.0min	Stop	Stop															
1.0ml/min																	
Flow rate:																	
Wavelength:	215nm																
Volume:	10µl																

## 3. Result

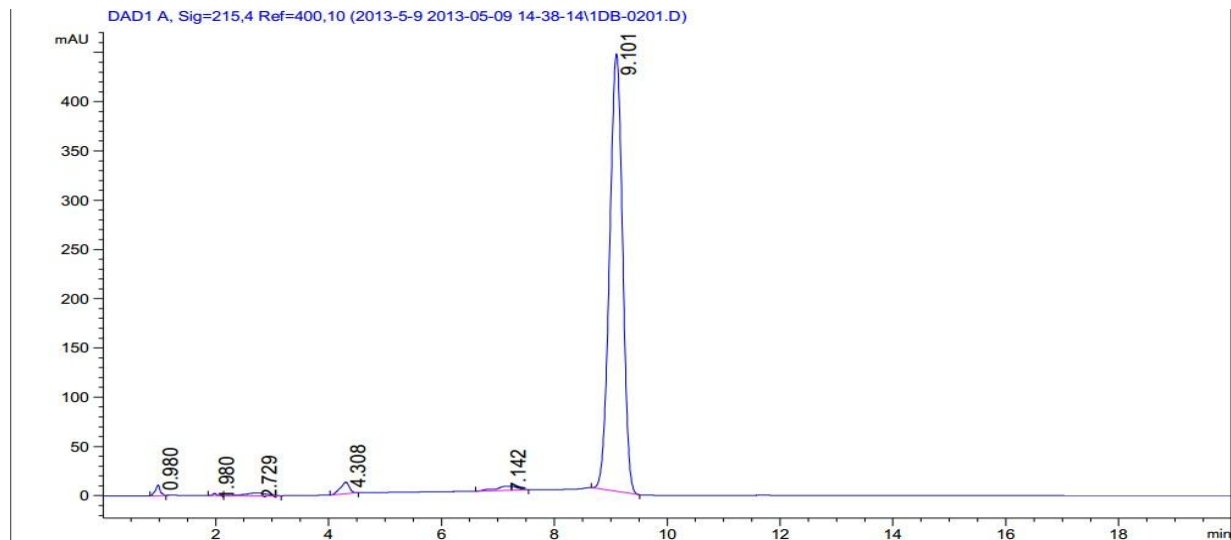

Rank	RetTime(mi)	Area(mAU*)	Area %
1	0.980	62.24716	0.8308
2	1.9802	10.18970	0.1360
3	2.729	71.48685	0.9541
4	4.308	133.11646	1.7766
5	7.142	109.83662	1.4659
6	9.101	7105.99756	94.8367