

High Performance Liquid Chromatography

Analysis Information

Product Name: PIK-75 HCl

Operator: David

Injection Date: 4/11/2020 3:45:22 AM

Batch No.: 2

HPLC Condition

Column : ZORBAX Eclipse Pluse C18 3.5 μ m 4.6mmx100mm

Solvent A: H2O+0.1%TFA

Solvent B: ACN+0.1%TFA

Gradient:


Time	A	B
0.0min	80%	20%
2.0min	80%	20%
7.0min	5%	95%
10.00min	0%	100%
12.00min	0%	100%
15.00min	Stop	Stop

Flow rate: 1mL/min

Wavelength: 270nm

Volume: 5 μ l

Result

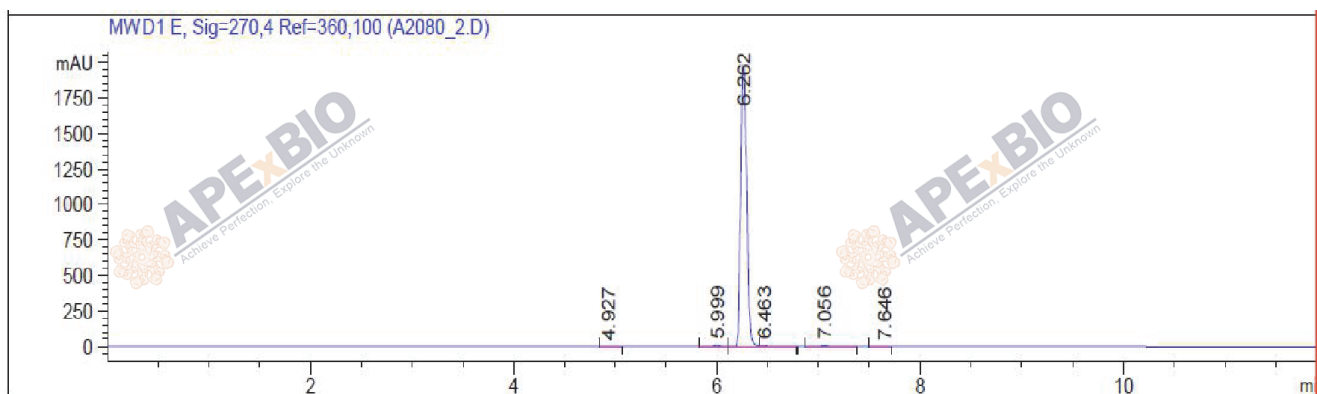

Rank	RetTime(min)	Area(mAU*s)	Area %
1	4.927	2.20490	0.0267
2	5.999	29.91683	0.3622
3	6.262	8191.81885	99.1705
4	6.463	9.89867	0.1198
5	7.056	24.94378	0.3020
6	7.646	1.55296	0.0188

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEXBIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com