

High Performance Liquid Chromatography

Analysis Information

Product Name: PIK-75 HCl

Operator: David

Injection Date: 4/11/2020 4:01:54 AM

Batch No.: 3

HPLC Condition

Column : ZORBAX Eclipse Pluse C18 3.5 μ m 4.6mmx100mm

Solvent A: H2O+0.1%TFA

Solvent B: ACN+0.1%TFA

Gradient:


Time	A	B
0.0min	80%	20%
2.0min	80%	20%
7.0min	5%	95%
10.00min	0%	100%
12.00min	0%	100%
15.00min	Stop	Stop

Flow rate: 1mL/min

Wavelength: 270nm

Volume: 5 μ l

Result

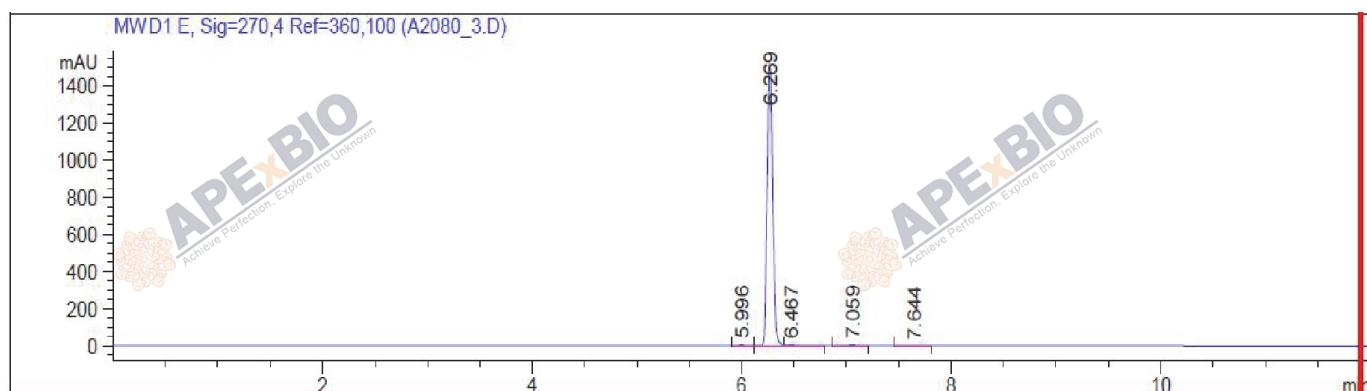

Rank	RetTime(min)	Area(mAU*s)	Area %
1	5.996	9.41771	0.1666
2	6.269	5620.66846	99.4021
3	6.467	10.04450	0.1776
4	7.059	11.98759	0.2120
5	7.644	2.35639	0.0417

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APExBIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com