

High Performance Liquid Chromatography

Analysis Information

Product Name: PPACK Dihydrochloride

Operator: David

Injection Date: 1/17/2022 5:52:47 PM

Batch No.: 2

HPLC Condition

Column : Athena C18, 3 μ m, 2.1mm $\times$ 100 mm

Solvent A: ACN+0.1%TFA

Solvent B: H2O+0.1%TFA


Gradient:

Time	A	B
0.0min	0%	100%
2.0min	0%	100%
7.0min	95%	5%
10.0min	95%	5%
10.0min	Stop	Stop

Flow rate: 0.45ml/min

Wavelength: 210nm

Volume: 3 μ l

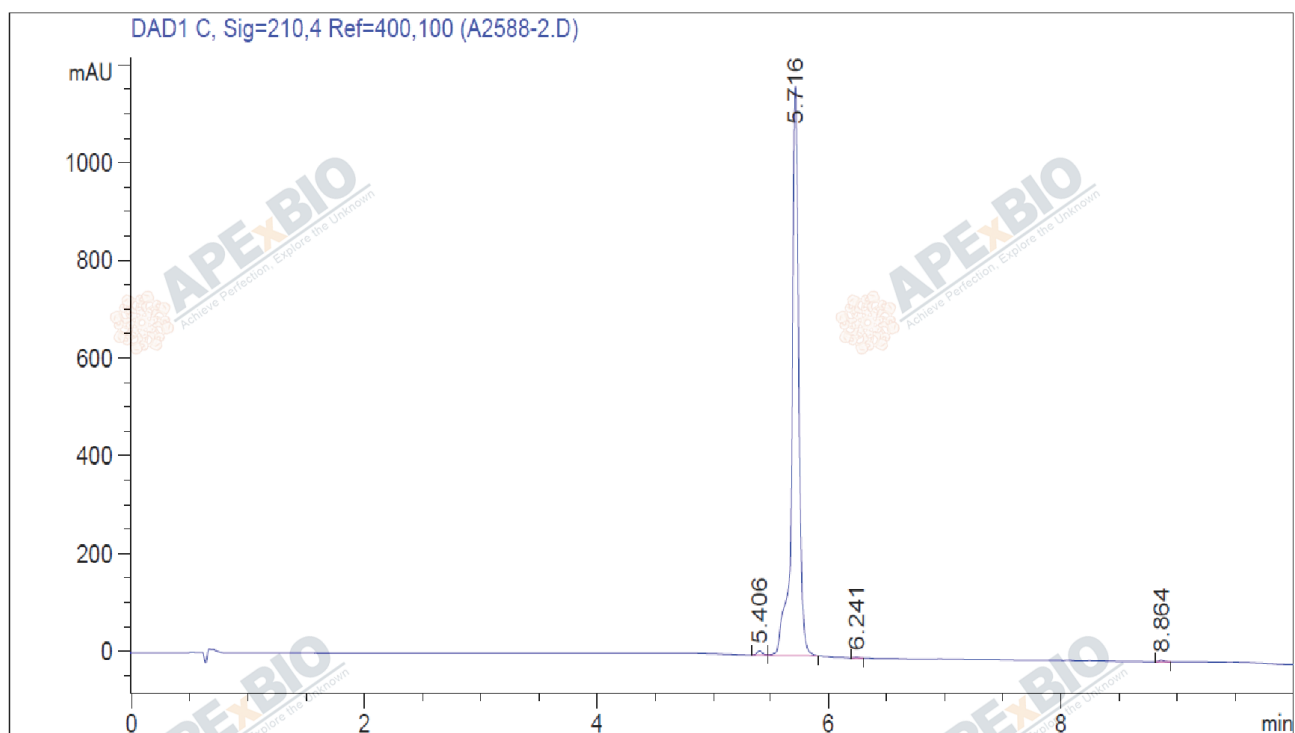

Rank	RetTime(min)	Area(mAU*s)	Area %
1	5.406	30.18791	0.6166
2	5.716	4851.87451	99.1092
3	6.241	3.70385	0.0757
4	8.864	9.71668	0.1985

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APExBIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

