

1. Analysis Information

Product Name:	ABT-263 (Navitoclax)
Operator:	David
Injection Date:	12/15/2016 01:22:18 PM
Inj. Volume:	1
Batch No.:	16


2. Acquisition Parameter

Probe:	ESI
Gas Temp:	350°C
Gas Flow:	11L/min
Nebulizer:	50psi
VCap:	4000v
Fragmentor:	70v
Reference:	m/z 121.050873, 922.009798
T.Flow:	0.3ml/min
B.conc:	20% H ₂ O/80% ACN

3. Result

20161215-B1-1213 10 (0.165)

1: Scan ES+
1.17e8

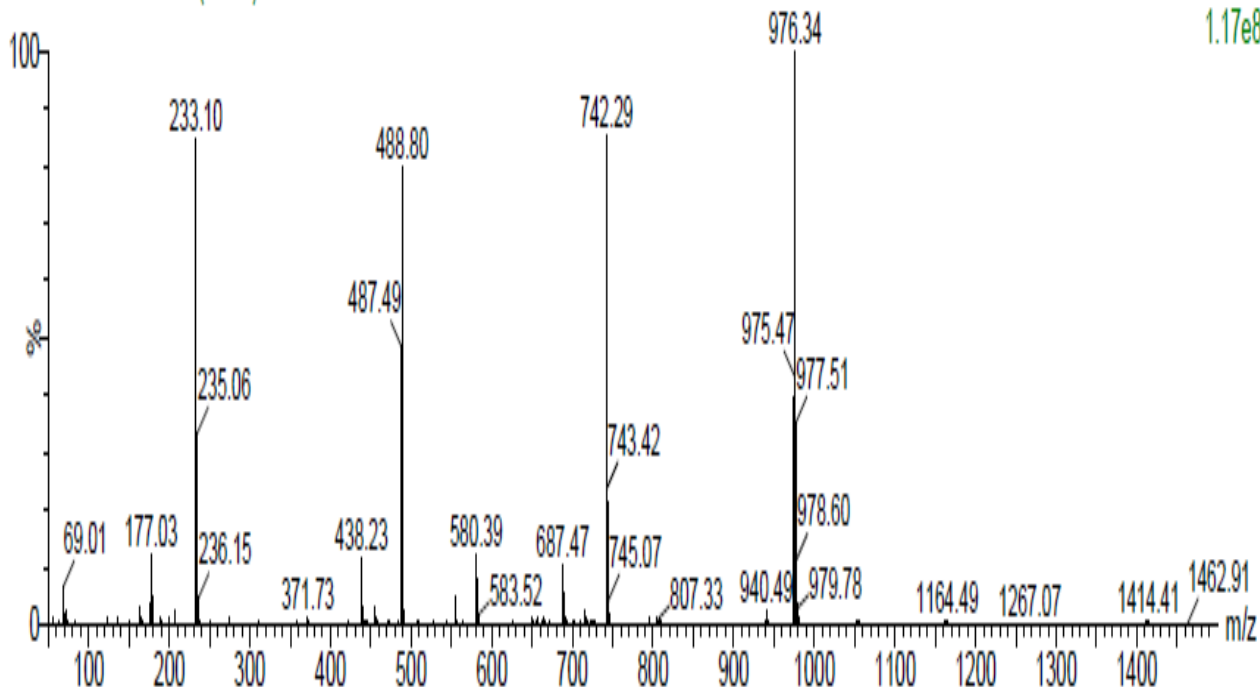

Molecular Weight:	974.61
m/z(M+2H) Base Peak :	976.47
m/z(M+H) Base Peak :	975.47