

High Performance Liquid Chromatography

Analysis Information

Product Name: CHIR-99021 (CT99021)

Operator: David

Injection Date: 11/18/2021 7:46:24 PM

Batch No.: 4

HPLC Condition

Column : Athena C18, 3 μ m, 2.1mm $\times$ 100 mm

Solvent A: ACN+0.1%TFA

Solvent B: H2O+0.1%TFA


Gradient:

Time	A	B
0.0min	0%	100%
1.5min	0%	100%
6.0min	95%	5%
9.0min	95%	5%
9.0min	Stop	Stop

Flow rate: 0.46ml/min

Wavelength: 276nm

Volume: 3 μ l

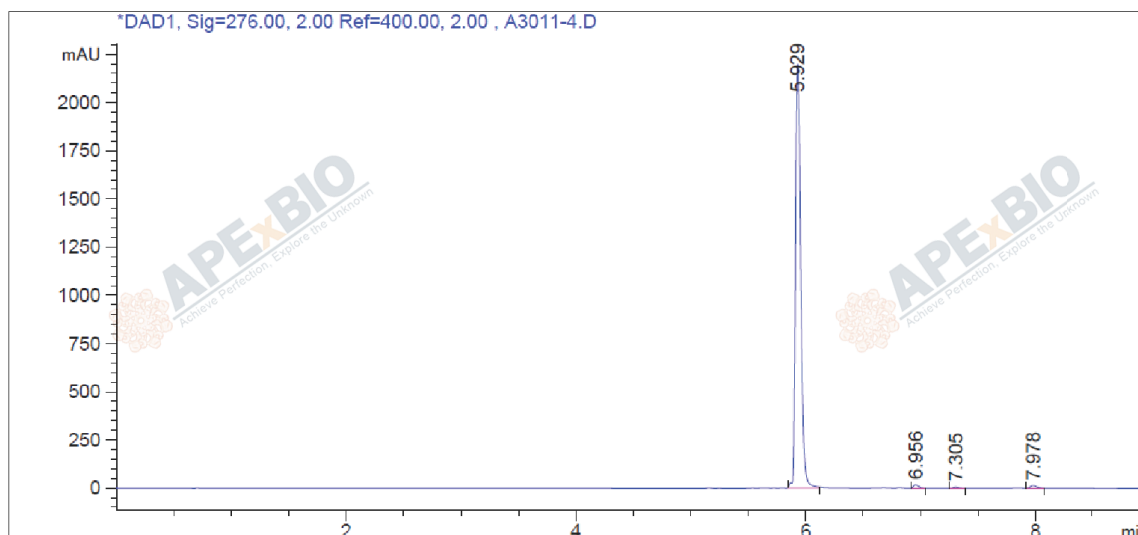

Rank	RetTime(min)	Area(mAU*s)	Area %
1	5.929	6908.77979	98.3271
2	6.956	50.96911	0.7254
3	7.305	18.90433	0.2690
4	7.978	47.67279	0.6785

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com