

High Performance Liquid Chromatography

Analysis Information

Product Name: PLX-4720

Operator: David

Injection Date: 4/11/2020 9:32:56 AM

Batch No.: 1

HPLC Condition

Column : ZORBAX Eclipse Pluse C18 3.5 μ m 4.6mmx100mm

Solvent A: H2O+0.1%TFA

Solvent B: ACN+0.1%TFA

Gradient:


Time	A	B
0.0min	80%	20%
2.0min	80%	20%
7.0min	5%	95%
10.00min	0%	100%
12.00min	0%	100%
15.00min	Stop	Stop

Flow rate: 1mL/min

Wavelength: 254nm

Volume: 3 μ l

Result

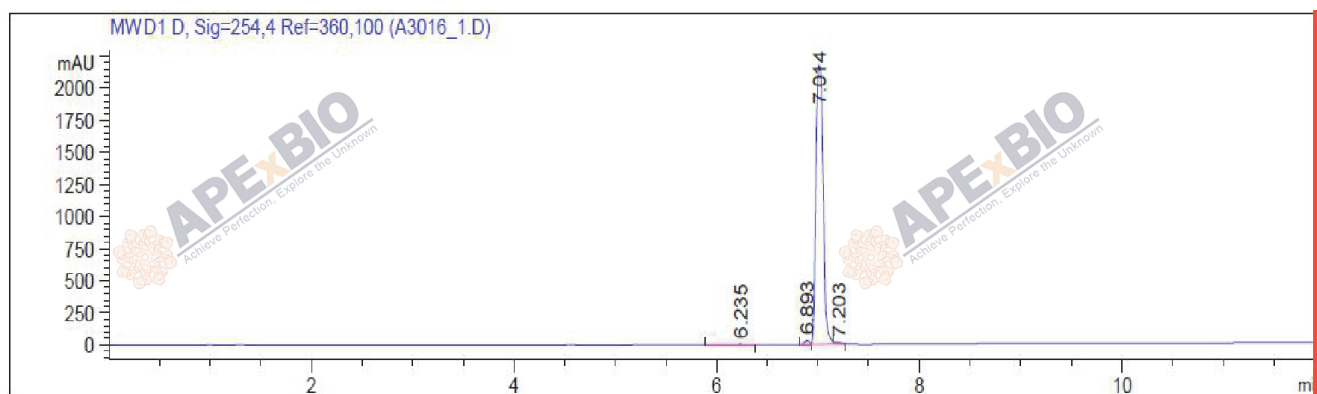

Rank	RetTime(min)	Area(mAU*s)	Area %
1	6.235	20.07540	0.1821
2	6.893	94.39124	0.8561
3	7.014	1.08821e4	98.7015
4	7.203	28.69549	0.2603

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com