

## Mass Spectrometry

### Analysis Information


**Product Name:** AM095  
**Operator:** David  
**Injection Date:** 3/6/2019 2:25:32 PM  
**Inj. Volume:** 1  
**Batch No.:** 3

### Acquisition Parameter

**Probe:** ESI  
**Gas Temp:** 350°C  
**Gas Flow:** 11L/min  
**Nebulizer:** 50psi  
**VCap:** 4000v  
**Fragmentor:** 70v  
**Reference:** m/z 121.050873, 922.009798  
**T.Flow:** 0.3ml/min  
**B.conc:** 20%H<sub>2</sub>O/80%ACN

# Result

Sample Name	0306	Position	P2-A5	Instrument Name	Instrument 1
User Name		Inj Vol	Unknown / Injection Program	InjPosition	
Sample Type	Sample	IRM Calibration Status	Success	Data Filename	A3166-3-POS.d
ACQ Method	20190215-HPLC-POS.m	Comment		Acquired Time	3/6/2019 2:25:32 PM (UTC+08:00)

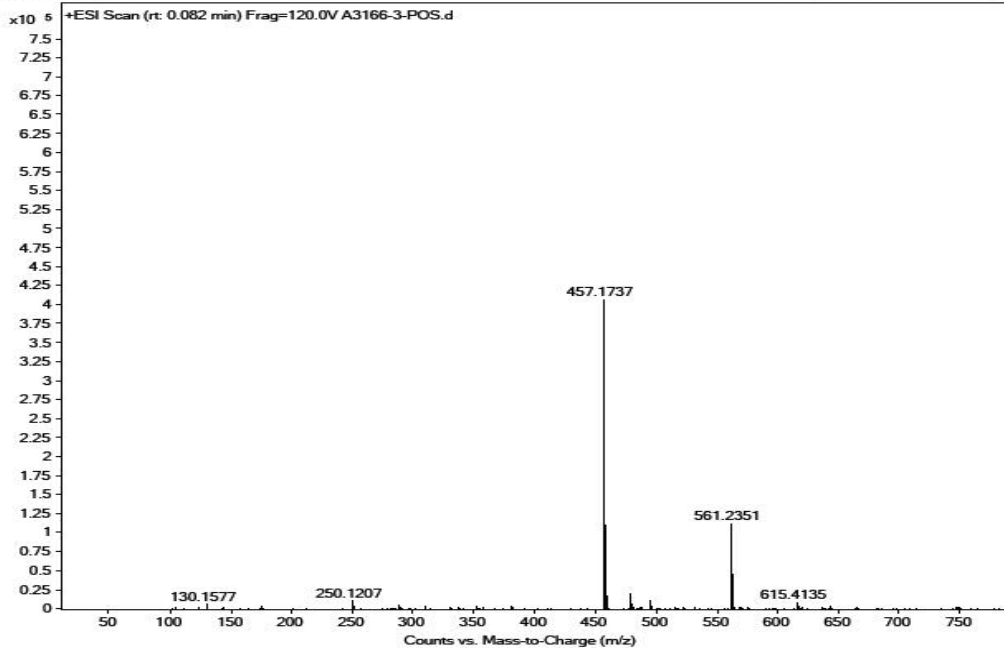

**Molecular Weight:** 478.47

**m/z([M-Na+2H]-) Base Peak:** 457.1737

**m/z([M+2Na+2H<sub>2</sub>O]+) Base Peak:** 561.2351

## Caution

**FOR RESEARCH PURPOSES ONLY.**

**NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.**

**APEX BIO Technology**

**www.apexbt.com**

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com