

High Performance Liquid Chromatography

1. Analysis Information

Product Name:	GS-9620
Operator:	David
Injection Date:	8/11/2015 9:51:25 AM
Batch No.:	1


2. HPLC Condition

Column:	Athena C18, 3 μ m, 2.1mm \times 100 mm
Solvent A:	0.1% H ₃ PO ₄ in 100% Acetonitrile
Solvent B:	0.1% H ₃ PO ₄ in 100% Water

Gradient:	Time	A	B
	0.0min	10%	90%
	3.5min	95%	5%
	8.0min	95%	5%
	9.0min	10%	90%
	10.0min	10%	90%
	10.0min	Stop	Stop

Flow rate:	0.4ml/min
Wavelength:	210nm
Volume:	10 μ l

3. Result

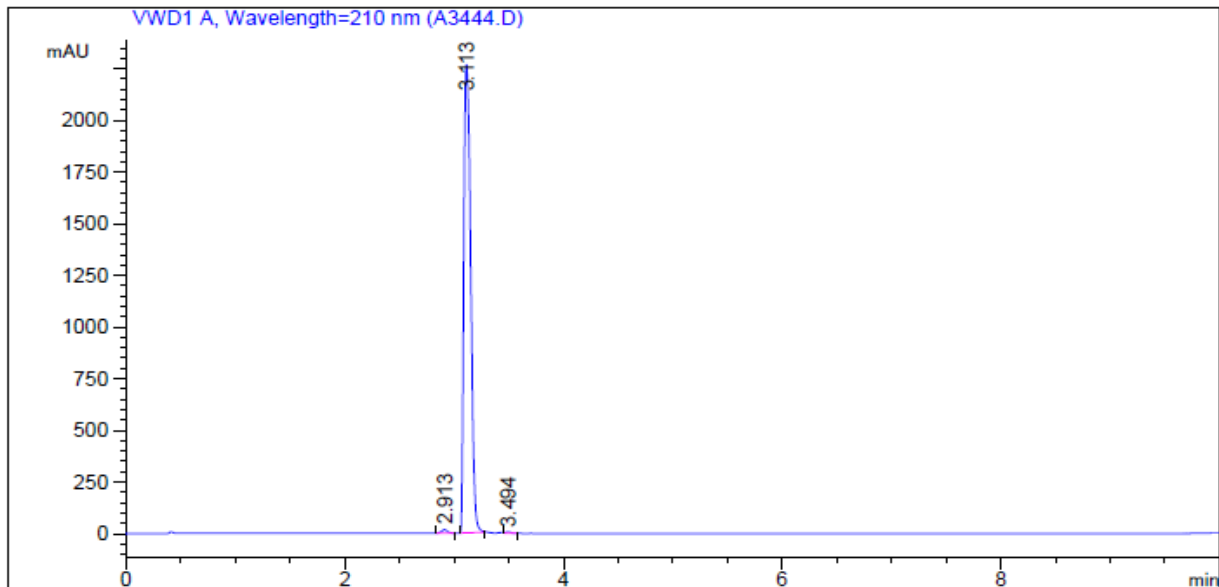

Rank	RetTime(min)	Area(mAU*s)	Area %
1	2.913	69.06212	0.6950
2	3.113	9850.09961	99.1301
3	3.494	17.37421	0.1749