

Mass Spectrometry

Analysis Information

Product Name: LCL161
Operator: David
Injection Date: 01/18/2017
Inj. Volume: 1
Batch No.: 2

Acquisition Parameter


Probe: ESI
Gas Temp: 350°C
Gas Flow: 11L/min
Nebulizer: 50psi
VCap: 4000v
Fragmentor: 70v
Reference: m/z 121.050873, 922.009798
T.Flow: 0.3ml/min
B.conc: 20%H₂O/80%ACN

Result

13:45:43NT-S20170116-069

20170118-1005342-46-0 10 (0.165)

1: Scan ES+
5.74e7

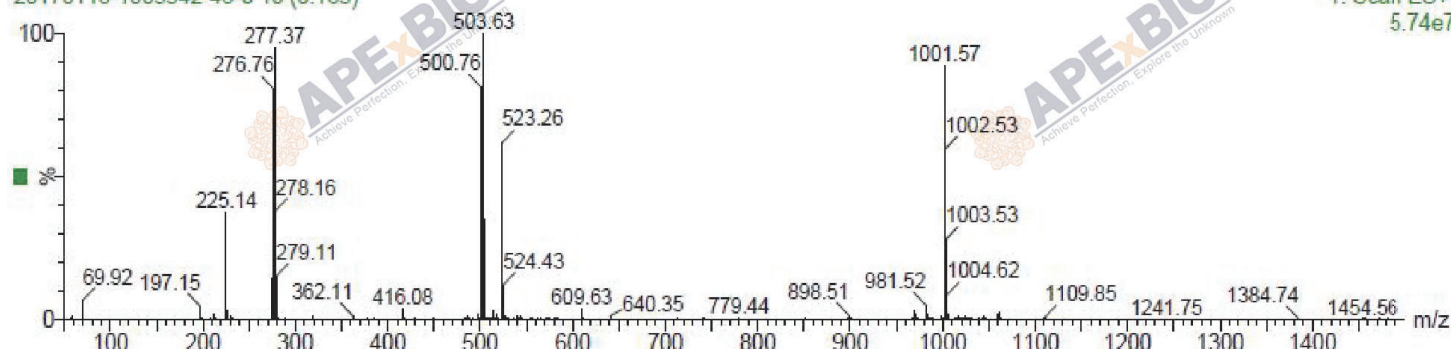

Molecular Weight: 500.63

m/z([M+3H]⁺) Base Peak: 503.63

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com