

High Performance Liquid Chromatography

Analysis Information

Product Name: SLx-2119

Operator: David

Injection Date: 12/15/2020 3:10:19 PM

Batch No.: 3

HPLC Condition

Column : ZORBAX Eclipse Pluse C18 3.5 μ m 4.6mmx100mm

Solvent A: H2O+0.1%TFA

Solvent B: ACN+0.1%TFA

Gradient:


Time	A	B
0.0min	80%	5%
2.0min	80%	5%
12.0min	5%	95%
13.0min	0%	100%
16.0min	0%	100%
16.0min	Stop	Stop

Flow rate: 1ml/min

Wavelength: 280nm

Volume: 5 μ l

Result

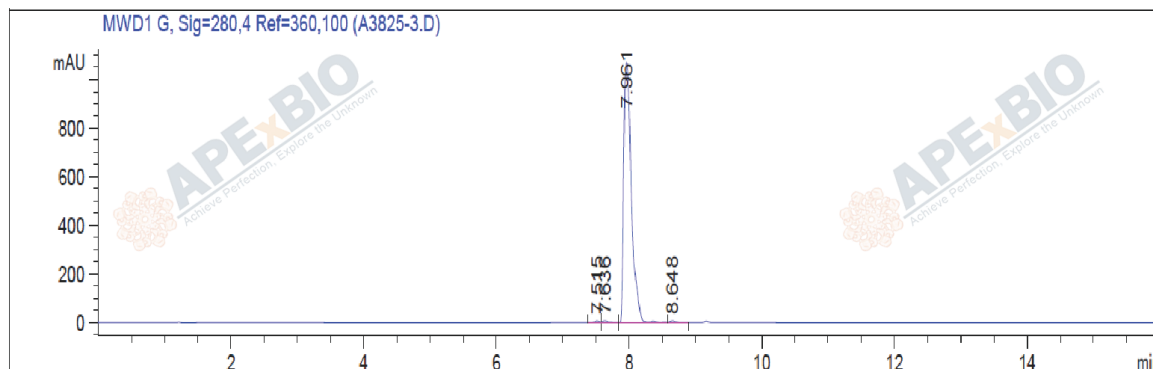

Rank	RetTime(min)	Area(mAU*s)	Area %
1	7.515	28.81362	0.3332
2	7.636	36.75769	0.4250
3	7.961	8544.77441	98.8000
4	8.648	38.20921	0.4418

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEx BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com