

High Performance Liquid Chromatography

Analysis Information

Product Name: MK-8245
Operator: David
Injection Date: 3/19/2019 6:09:15 PM
Batch No.: 2

HPLC Condition

Column : ZORBAX Eclipse Pluse C18 3.5 μ m 4.6mmx100mm

Solvent A: H2O+0.1%TFA

Solvent B: ACN+0.1%TFA

Gradient:

Time	A	B
0.0min	95%	5%
2.0min	95%	5%
7.0min	5%	95%
10.00min	0%	100%
12.00min	0%	100%
12.10min	95%	5%
15.00min	Stop	Stop


Flow rate: 1mL/min

Wavelength: 254nm

Volume:

3 μ l

Result

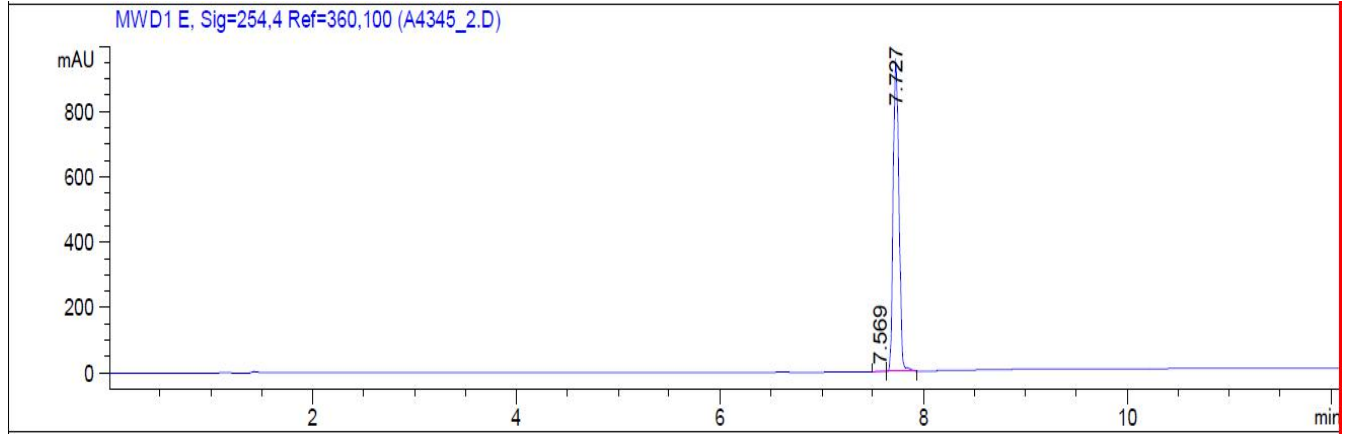

Rank	RetTime(min)	Area(mAU*s)	Area %
1	7.569	8.92410	0.2375
2	7.727	3749.34106	99.7625

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APExBIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com